

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035122.D
 Acq On : 11 Apr 2024 10:52
 Operator : SY/MD
 Sample : P2006-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	245897	256049	15.45%	2.241%
2	1.529	145	152	165	rVB	202162	242016	14.60%	2.118%
3	2.056	307	316	331	rBV	405534	581591	35.10%	5.090%
4	2.497	452	453	459	rBV2	337	240	0.01%	0.002%
5	2.558	470	472	473	rBV	689	282	0.02%	0.002%
6	2.613	487	489	492	rVB2	379	183	0.01%	0.002%
7	2.654	499	502	506	rBV2	320	317	0.02%	0.003%
8	2.838	551	559	566	rBV4	582	991	0.06%	0.009%
9	2.892	573	576	580	rVB2	263	123	0.01%	0.001%
10	2.954	592	595	596	rBV	250	152	0.01%	0.001%
11	2.982	602	604	607	rBV2	388	235	0.01%	0.002%
12	3.044	621	623	631	rVB3	388	446	0.03%	0.004%
13	3.079	631	634	637	rBV	167	141	0.01%	0.001%
14	3.124	642	648	649	rBV4	719	461	0.03%	0.004%
15	3.163	658	660	663	rBV	289	153	0.01%	0.001%
16	3.291	696	700	705	rBV2	257	298	0.02%	0.003%
17	3.372	721	725	726	rBV	208	122	0.01%	0.001%
18	3.400	730	734	737	rVV	359	285	0.02%	0.002%
19	3.484	758	760	766	rVB4	239	208	0.01%	0.002%
20	3.532	772	775	778	rBV2	167	119	0.01%	0.001%
21	3.584	785	791	795	rBV2	258	231	0.01%	0.002%
22	3.629	802	805	806	rBV	262	149	0.01%	0.001%
23	3.645	806	810	813	rVV2	338	277	0.02%	0.002%
24	3.735	835	838	840	rBV2	284	200	0.01%	0.002%
25	3.783	845	853	894	rBV	123668	361476	21.81%	3.164%
26	4.246	982	997	1028	rBV	251883	651775	39.33%	5.704%
27	4.606	1106	1109	1112	rBV3	625	606	0.04%	0.005%
28	4.667	1124	1128	1133	rBV3	354	405	0.02%	0.004%
29	4.719	1142	1144	1146	rBV2	503	228	0.01%	0.002%
30	4.748	1151	1153	1157	rVB2	392	215	0.01%	0.002%
31	4.953	1201	1217	1255	rBV2	624333	1657090	100.00%	14.503%
32	5.320	1329	1331	1332	rBV2	340	132	0.01%	0.001%
33	5.416	1359	1361	1363	rVB	462	174	0.01%	0.002%
34	5.429	1363	1365	1368	rBV2	231	166	0.01%	0.001%
35	5.532	1386	1397	1425	rBV	352882	738518	44.57%	6.463%
36	5.924	1517	1519	1520	rBV	460	195	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035122.D
 Acq On : 11 Apr 2024 10:52
 Operator : SY/MD
 Sample : P2006-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1525	1538	1567	rBV	364264	766548	46.26%	6.709%
38	6.342	1646	1649	1655	rVB2	466	303	0.02%	0.003%
39	6.375	1655	1659	1661	rBV3	625	445	0.03%	0.004%
40	6.442	1678	1680	1684	rVB	221	138	0.01%	0.001%
41	6.461	1684	1686	1687	rBV	369	163	0.01%	0.001%
42	6.494	1693	1696	1698	rBV2	393	198	0.01%	0.002%
43	6.564	1716	1718	1720	rBV2	354	206	0.01%	0.002%
44	6.590	1724	1726	1732	rVB3	698	532	0.03%	0.005%
45	6.622	1732	1736	1737	rBV2	342	244	0.01%	0.002%
46	6.674	1749	1752	1753	rBV	235	135	0.01%	0.001%
47	6.715	1762	1765	1766	rBV2	429	273	0.02%	0.002%
48	6.802	1789	1792	1795	rVB	281	208	0.01%	0.002%
49	6.831	1797	1801	1804	rVB3	415	262	0.02%	0.002%
50	6.857	1806	1809	1812	rBV2	353	217	0.01%	0.002%
51	6.876	1812	1815	1816	rBV3	429	257	0.02%	0.002%
52	6.912	1816	1826	1860	rBV	178879	350224	21.13%	3.065%
53	7.243	1918	1929	1955	rBV	695837	1241118	74.90%	10.862%
54	7.551	2017	2025	2052	rBV	120973	227127	13.71%	1.988%
55	7.870	2122	2124	2126	rBV2	392	175	0.01%	0.002%
56	7.966	2152	2154	2159	rVB3	596	332	0.02%	0.003%
57	7.992	2159	2162	2163	rBV	415	192	0.01%	0.002%
58	8.024	2163	2172	2214	rBV3	345442	762295	46.00%	6.672%
59	8.500	2317	2320	2324	rBV2	477	464	0.03%	0.004%
60	8.664	2369	2371	2374	rBV2	339	180	0.01%	0.002%
61	8.731	2389	2392	2393	rBV2	260	152	0.01%	0.001%
62	8.783	2398	2408	2433	rBV	551894	911051	54.98%	7.973%
63	9.008	2476	2478	2479	rBV	566	261	0.02%	0.002%
64	9.056	2491	2493	2499	rBV3	738	700	0.04%	0.006%
65	9.191	2532	2535	2536	rBV	360	219	0.01%	0.002%
66	9.233	2545	2548	2550	rBV2	644	387	0.02%	0.003%
67	9.249	2550	2553	2557	rVB2	560	393	0.02%	0.003%
68	9.384	2592	2595	2600	rVB3	547	382	0.02%	0.003%
69	9.423	2604	2607	2611	rBV3	299	229	0.01%	0.002%
70	9.468	2615	2621	2624	rVB2	615	358	0.02%	0.003%
71	9.487	2624	2627	2630	rBV2	914	728	0.04%	0.006%
72	9.551	2642	2647	2650	rBV3	463	439	0.03%	0.004%
73	9.574	2652	2654	2656	rVB2	396	146	0.01%	0.001%
74	9.619	2666	2668	2672	rVB2	367	184	0.01%	0.002%
75	9.648	2675	2677	2685	rVB2	395	440	0.03%	0.004%
76	9.696	2690	2692	2693	rBV2	237	126	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035122.D
 Acq On : 11 Apr 2024 10:52
 Operator : SY/MD
 Sample : P2006-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.738	2703	2705	2709	rBV2	304	186	0.01%	0.002%
78	9.789	2715	2721	2722	rBV	374	228	0.01%	0.002%
79	9.815	2726	2729	2731	rBV	264	164	0.01%	0.001%
80	9.873	2737	2747	2751	rBV3	772	1229	0.07%	0.011%
81	9.915	2758	2760	2765	rVB	350	232	0.01%	0.002%
82	9.947	2766	2770	2773	rBV2	276	219	0.01%	0.002%
83	10.149	2821	2833	2863	rBV	491584	793405	47.88%	6.944%
84	10.641	2984	2986	2988	rBV2	340	181	0.01%	0.002%
85	10.680	2997	2998	3002	rBV3	218	137	0.01%	0.001%
86	10.763	3021	3024	3026	rVB2	387	154	0.01%	0.001%
87	10.812	3036	3039	3041	rBV	365	184	0.01%	0.002%
88	11.030	3105	3107	3110	rBV2	208	129	0.01%	0.001%
89	11.085	3122	3124	3127	rBV	303	178	0.01%	0.002%
90	11.185	3144	3155	3186	rBV	493392	790423	47.70%	6.918%
91	11.497	3249	3252	3254	rBV2	279	218	0.01%	0.002%
92	11.558	3259	3271	3297	rBV	667058	1058180	63.86%	9.261%
93	12.021	3413	3415	3420	rBV3	452	363	0.02%	0.003%
94	12.152	3452	3456	3459	rBV2	580	507	0.03%	0.004%
95	12.352	3514	3518	3521	rBV3	660	404	0.02%	0.004%
96	12.387	3524	3529	3532	rBV2	604	528	0.03%	0.005%
97	12.651	3608	3611	3614	rBV2	332	157	0.01%	0.001%
98	13.300	3809	3813	3814	rBV3	607	529	0.03%	0.005%
99	13.355	3828	3830	3835	rBV2	464	492	0.03%	0.004%
100	13.448	3852	3859	3871	rBV2	7125	12972	0.78%	0.114%




Sum of corrected areas: 11426079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035122.D
Acq On : 11 Apr 2024 10:52
Operator : SY/MD
Sample : P2006-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

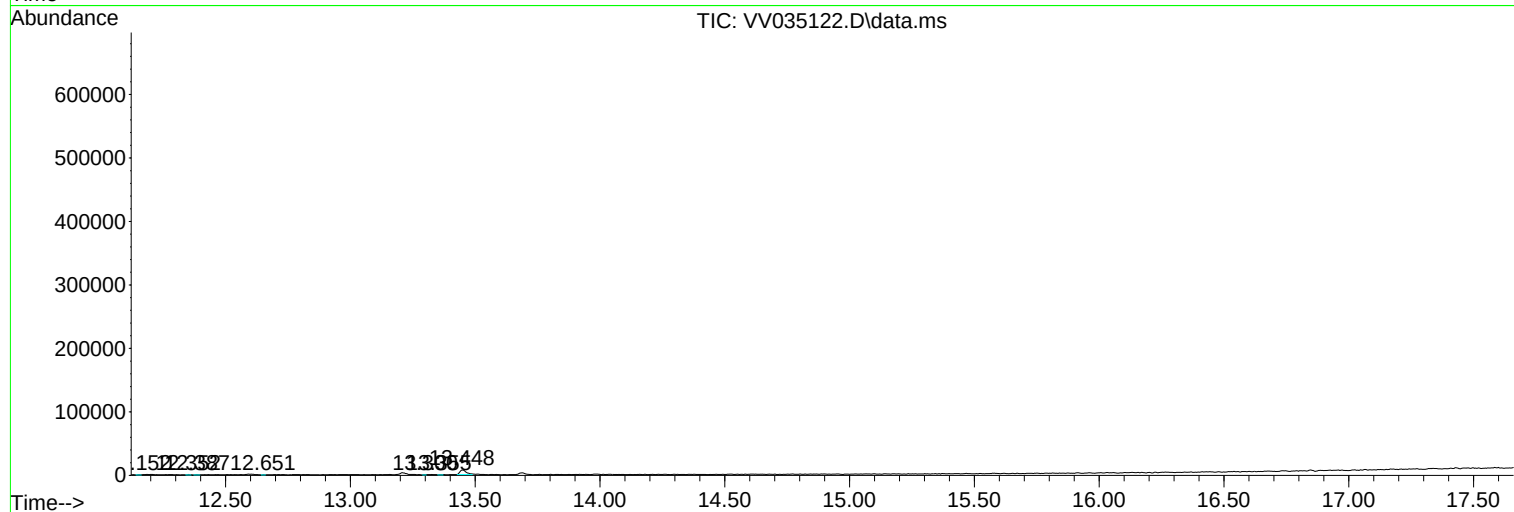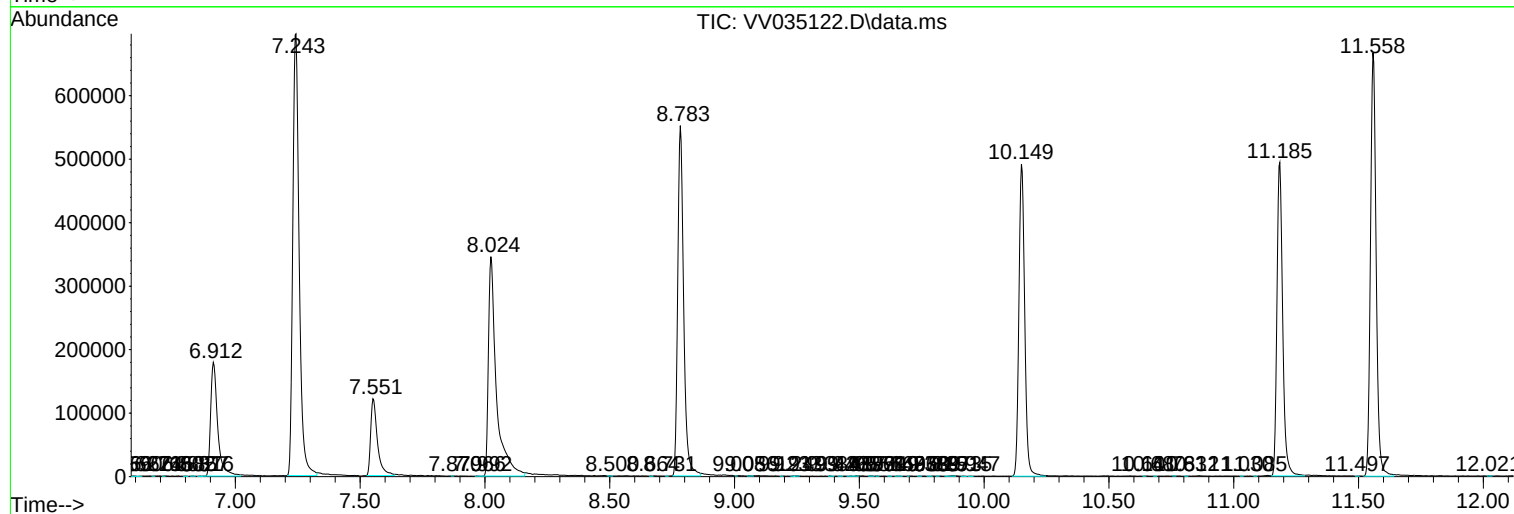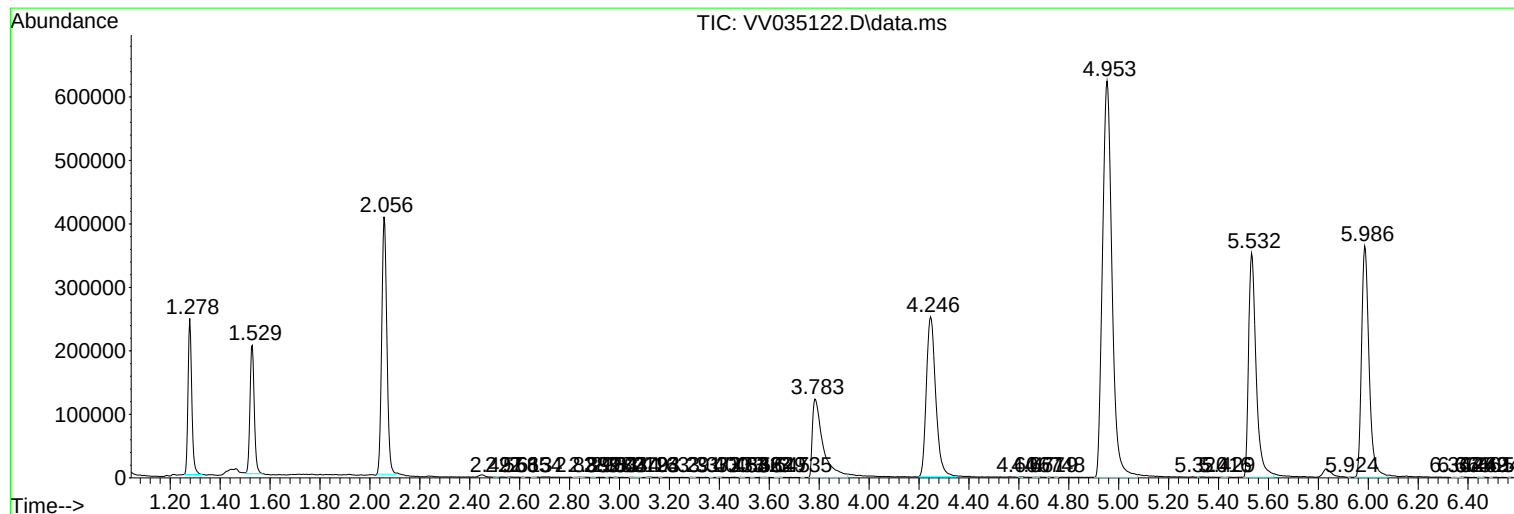

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035122.D
Acq On : 11 Apr 2024 10:52
Operator : SY/MD
Sample : P2006-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035122.D
Acq On : 11 Apr 2024 10:52
Operator : SY/MD
Sample : P2006-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------