

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035123.D
 Acq On : 11 Apr 2024 11:16
 Operator : SY/MD
 Sample : P2007-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	253157	266021	15.88%	2.291%
2	1.529	145	152	170	rVB	211425	252166	15.05%	2.172%
3	2.056	307	316	332	rBV	410034	593500	35.43%	5.111%
4	2.413	425	427	430	rBV2	681	483	0.03%	0.004%
5	2.542	465	467	468	rBV2	346	101	0.01%	0.001%
6	2.654	499	502	504	rBV2	444	284	0.02%	0.002%
7	2.867	566	568	569	rBV	240	79	0.00%	0.001%
8	2.947	589	593	596	rVB3	313	212	0.01%	0.002%
9	3.005	607	611	612	rBV	304	164	0.01%	0.001%
10	3.037	619	621	624	rVB2	347	158	0.01%	0.001%
11	3.108	640	643	646	rBV3	384	245	0.01%	0.002%
12	3.217	675	677	682	rBV2	243	214	0.01%	0.002%
13	3.294	699	701	704	rVB	372	164	0.01%	0.001%
14	3.314	704	707	711	rBV3	413	365	0.02%	0.003%
15	3.413	737	738	740	rBV	249	103	0.01%	0.001%
16	3.452	748	750	751	rBV	167	96	0.01%	0.001%
17	3.539	775	777	778	rBV	117	31	0.00%	0.000%
18	3.580	786	790	793	rBV	318	257	0.02%	0.002%
19	3.593	793	794	797	rVV2	225	113	0.01%	0.001%
20	3.625	803	804	805	rBV	239	74	0.00%	0.001%
21	3.680	819	821	823	rBV	204	103	0.01%	0.001%
22	3.786	846	854	897	rBV	123026	361887	21.60%	3.116%
23	4.246	982	997	1035	rBV	257741	663251	39.59%	5.712%
24	4.690	1131	1135	1137	rBV3	521	423	0.03%	0.004%
25	4.735	1147	1149	1152	rBV3	515	213	0.01%	0.002%
26	4.857	1184	1187	1188	rBV2	466	224	0.01%	0.002%
27	4.953	1201	1217	1248	rBV2	636635	1675235	100.00%	14.426%
28	5.268	1312	1315	1318	rBV4	889	720	0.04%	0.006%
29	5.494	1383	1385	1386	rBV	614	254	0.02%	0.002%
30	5.532	1387	1397	1432	rVV	365735	769137	45.91%	6.623%
31	5.985	1525	1538	1569	rBV	372296	771997	46.08%	6.648%
32	6.365	1654	1656	1659	rBV3	389	274	0.02%	0.002%
33	6.474	1688	1690	1691	rBV	257	84	0.01%	0.001%
34	6.506	1697	1700	1703	rVB2	467	284	0.02%	0.002%
35	6.555	1712	1715	1721	rBV2	429	426	0.03%	0.004%
36	6.577	1721	1722	1725	rBV2	157	91	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035123.D
 Acq On : 11 Apr 2024 11:16
 Operator : SY/MD
 Sample : P2007-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.593	1725	1727	1728	rBV	194	71	0.00%	0.001%
38	6.625	1736	1737	1738	rBV	349	92	0.01%	0.001%
39	6.635	1738	1740	1742	rVV2	411	234	0.01%	0.002%
40	6.648	1742	1744	1748	rVB3	591	403	0.02%	0.003%
41	6.702	1757	1761	1762	rBV2	401	292	0.02%	0.003%
42	6.712	1762	1764	1766	rVV	266	118	0.01%	0.001%
43	6.725	1766	1768	1770	rVB2	405	185	0.01%	0.002%
44	6.738	1770	1772	1774	rBV	190	96	0.01%	0.001%
45	6.770	1779	1782	1784	rBV2	284	193	0.01%	0.002%
46	6.809	1792	1794	1796	rBV	240	98	0.01%	0.001%
47	6.821	1796	1798	1799	rBV	194	67	0.00%	0.001%
48	6.857	1808	1809	1810	rBV	148	41	0.00%	0.000%
49	6.870	1810	1813	1816	rVB	326	226	0.01%	0.002%
50	6.911	1816	1826	1852	rBV	179980	348743	20.82%	3.003%
51	7.243	1918	1929	1961	rBV	717584	1274479	76.08%	10.975%
52	7.551	2017	2025	2055	rBV	122899	228816	13.66%	1.970%
53	7.799	2099	2102	2106	rBV4	557	389	0.02%	0.003%
54	7.857	2117	2120	2121	rBV2	331	165	0.01%	0.001%
55	7.899	2131	2133	2134	rBV	304	88	0.01%	0.001%
56	7.944	2145	2147	2151	rVB4	497	274	0.02%	0.002%
57	7.963	2151	2153	2155	rBV2	422	194	0.01%	0.002%
58	8.024	2163	2172	2217	rBV3	341110	768985	45.90%	6.622%
59	8.638	2360	2363	2365	rBV2	358	196	0.01%	0.002%
60	8.654	2365	2368	2371	rBV2	419	298	0.02%	0.003%
61	8.783	2397	2408	2437	rBV	564507	942609	56.27%	8.117%
62	9.050	2490	2491	2494	rBV3	574	304	0.02%	0.003%
63	9.156	2522	2524	2527	rVB	371	183	0.01%	0.002%
64	9.178	2527	2531	2533	rBV	292	234	0.01%	0.002%
65	9.204	2536	2539	2540	rBV	387	163	0.01%	0.001%
66	9.246	2550	2552	2554	rBV	518	242	0.01%	0.002%
67	9.355	2585	2586	2588	rVB	375	137	0.01%	0.001%
68	9.368	2588	2590	2591	rBV	389	186	0.01%	0.002%
69	9.397	2598	2599	2602	rVB2	242	73	0.00%	0.001%
70	9.419	2602	2606	2608	rBV3	437	392	0.02%	0.003%
71	9.718	2697	2699	2701	rBV2	229	108	0.01%	0.001%
72	9.747	2705	2708	2709	rBV2	126	74	0.00%	0.001%
73	9.767	2712	2714	2716	rVB	302	107	0.01%	0.001%
74	9.786	2716	2720	2725	rVB3	230	181	0.01%	0.002%
75	9.905	2756	2757	2760	rBV	266	121	0.01%	0.001%
76	9.931	2760	2765	2769	rVB2	431	427	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035123.D
 Acq On : 11 Apr 2024 11:16
 Operator : SY/MD
 Sample : P2007-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.950	2769	2771	2774	rBV2	359	204	0.01%	0.002%
78	9.992	2783	2784	2788	rVB2	414	246	0.01%	0.002%
79	10.046	2799	2801	2803	rBV2	297	132	0.01%	0.001%
80	10.082	2809	2812	2814	rBV	230	159	0.01%	0.001%
81	10.098	2814	2817	2821	rBV2	219	188	0.01%	0.002%
82	10.149	2821	2833	2858	rBV	497274	792383	47.30%	6.824%
83	10.516	2943	2947	2949	rBV2	335	285	0.02%	0.002%
84	10.567	2958	2963	2964	rBV	236	209	0.01%	0.002%
85	10.593	2969	2971	2973	rBV	266	156	0.01%	0.001%
86	10.648	2986	2988	2990	rBV	320	152	0.01%	0.001%
87	10.670	2993	2995	2996	rBV	155	50	0.00%	0.000%
88	10.706	3004	3006	3010	rBV2	335	283	0.02%	0.002%
89	11.030	3104	3107	3110	rBV3	315	220	0.01%	0.002%
90	11.046	3110	3112	3113	rBV3	340	145	0.01%	0.001%
91	11.127	3135	3137	3138	rBV2	523	242	0.01%	0.002%
92	11.185	3144	3155	3187	rBV	519184	820128	48.96%	7.063%
93	11.426	3227	3230	3231	rBV	475	277	0.02%	0.002%
94	11.558	3259	3271	3291	rBV	665304	1064751	63.56%	9.169%
95	12.152	3454	3456	3459	rBV	436	316	0.02%	0.003%
96	12.275	3490	3494	3495	rBV	314	201	0.01%	0.002%
97	12.516	3567	3569	3571	rBV	329	139	0.01%	0.001%
98	12.599	3587	3595	3601	rBV4	906	1468	0.09%	0.013%
99	13.165	3768	3771	3774	rBV	376	350	0.02%	0.003%




Sum of corrected areas: 11612401

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035123.D
Acq On : 11 Apr 2024 11:16
Operator : SY/MD
Sample : P2007-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

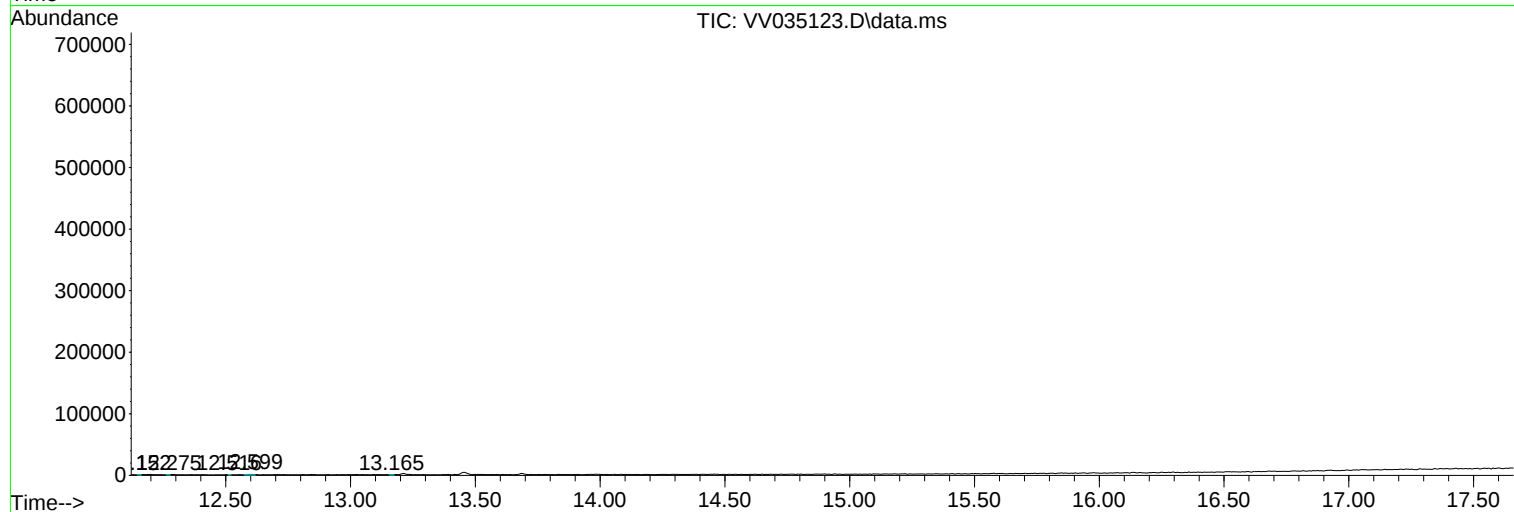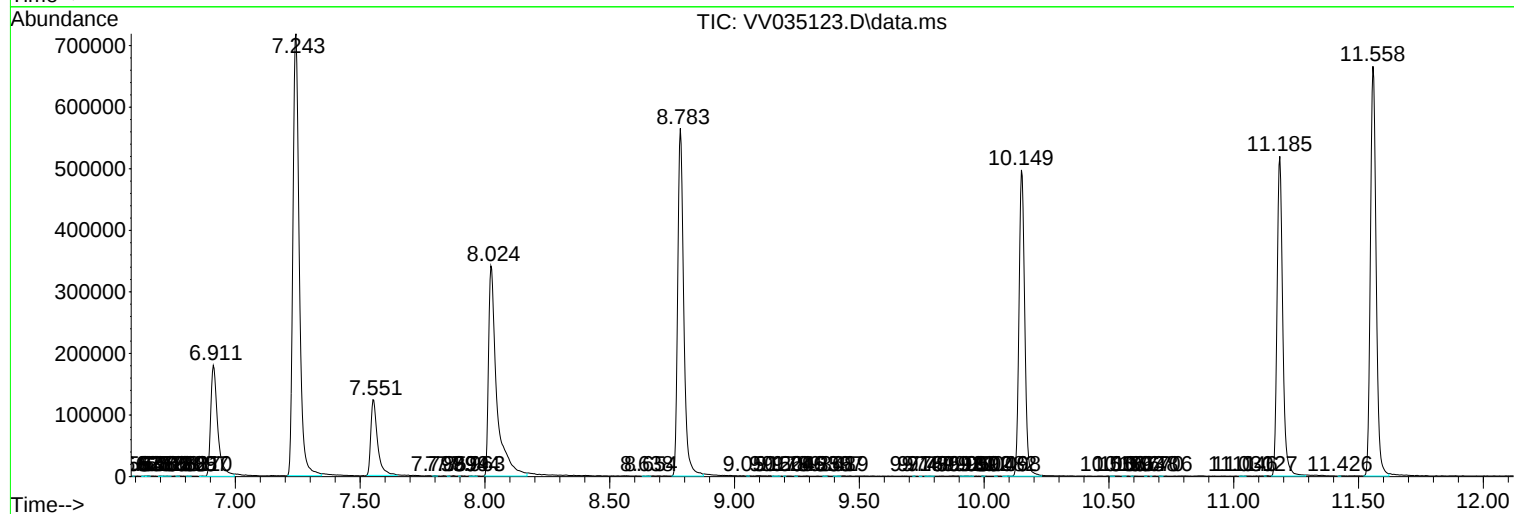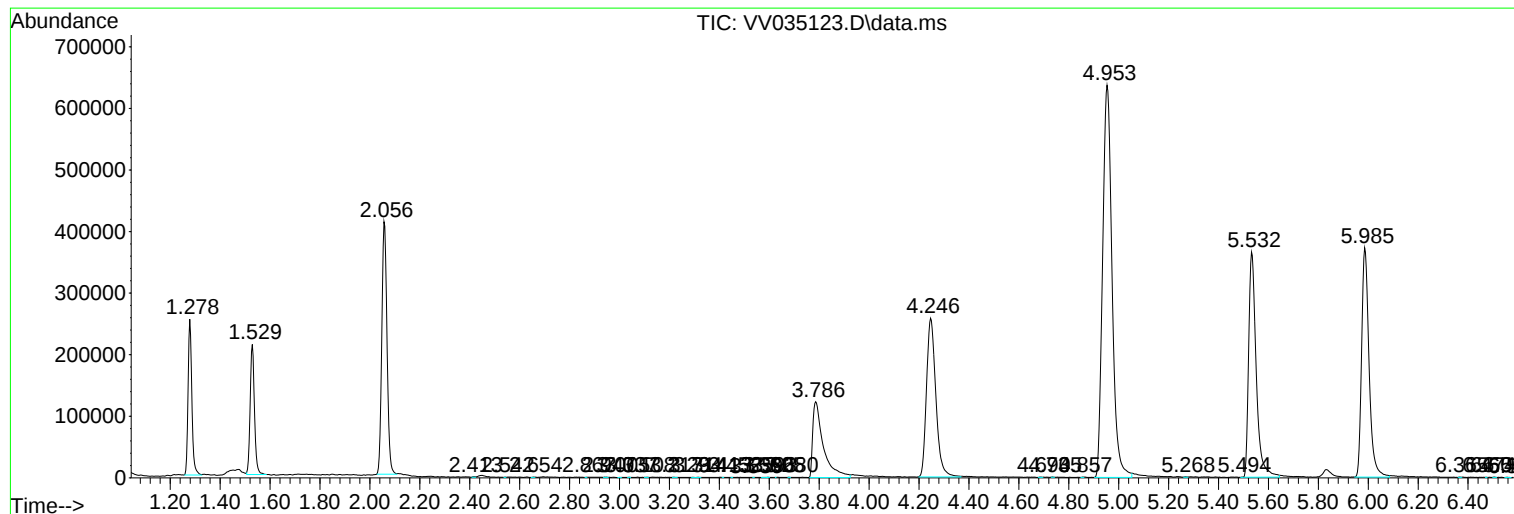

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035123.D
Acq On : 11 Apr 2024 11:16
Operator : SY/MD
Sample : P2007-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035123.D
Acq On : 11 Apr 2024 11:16
Operator : SY/MD
Sample : P2007-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc