
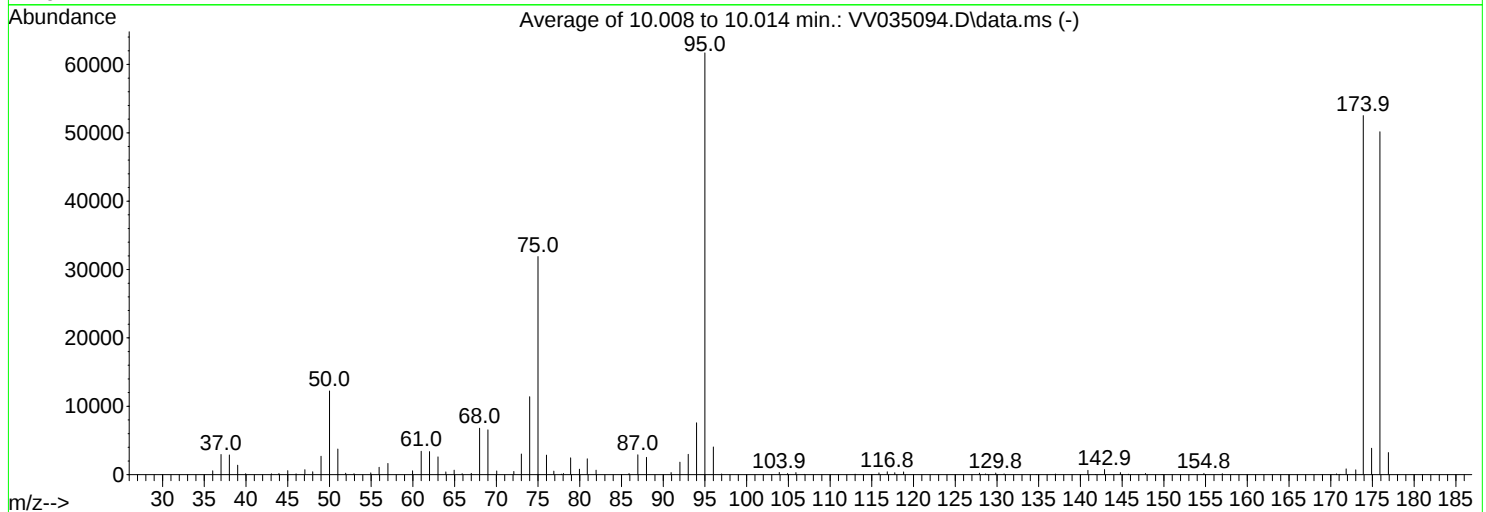


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035094.D
Acq On : 10 Apr 2024 08:28
Operator : SY/MD
Sample : BFB284
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB284

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Wed Apr 10 04:53:36 2024

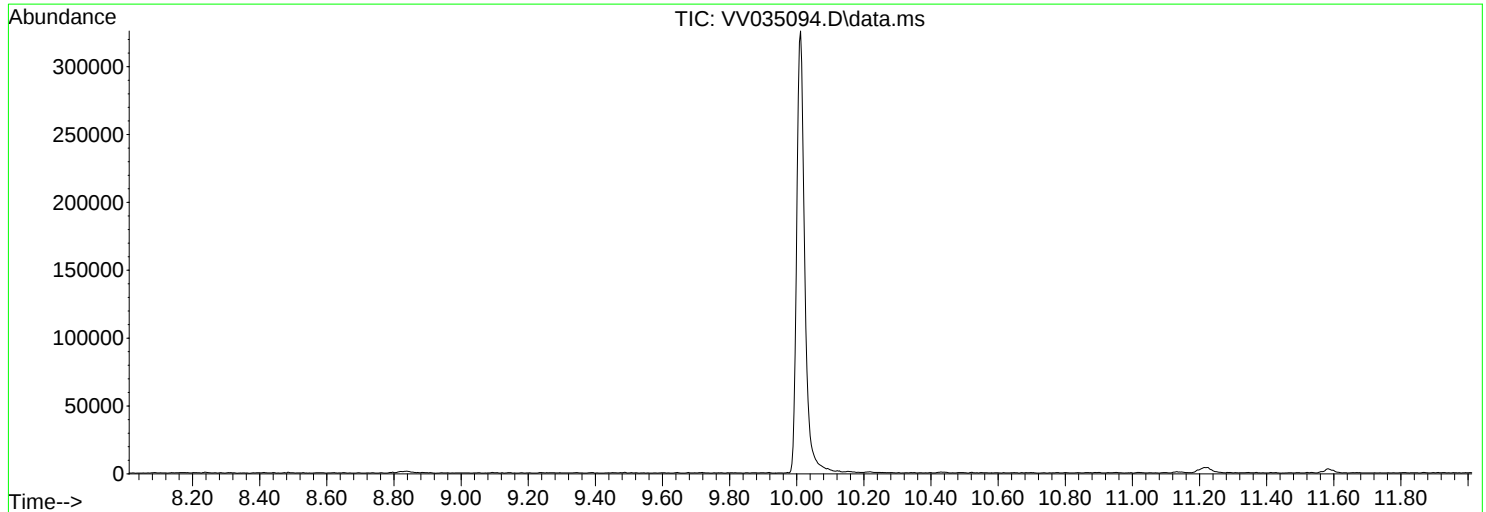

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	12246	PASS
75	95	30	80	51.7	31888	PASS
95	95	100	100	100.0	61693	PASS
96	95	5	9	6.6	4048	PASS
173	174	0.00	2	1.3	702	PASS
174	95	50	120	85.1	52517	PASS
175	174	5	9	7.4	3862	PASS
176	174	95	105	95.5	50144	PASS
177	176	5	10	6.4	3226	PASS

m/z	Abundance
40.00	174.0
41.00	102.0
44.00	562.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	577.0
37.00	3050.0
38.00	2930.0
39.00	1332.0
39.90	309.0
43.00	129.0
44.00	726.0
45.00	598.0
46.00	158.0
47.00	722.0
48.00	403.0
49.00	2834.0
50.00	12417.0
51.00	3883.0
51.90	217.0
53.00	163.0
54.90	246.0
56.00	1184.0
57.00	1748.0
60.00	652.0
61.00	3601.0
62.00	3366.0
63.00	2634.0
63.90	422.0
64.90	609.0
65.90	116.0
67.00	235.0
68.00	6921.0
69.00	6708.0
70.00	525.0
72.10	461.0
73.00	2993.0
74.00	11445.0
75.00	32640.0
76.00	3030.0
76.90	500.0
77.80	245.0
78.90	2448.0
80.00	795.0
80.90	2293.0
81.90	679.0
85.90	139.0
87.00	2990.0
88.00	2595.0
90.90	292.0
92.00	1830.0
93.00	3019.0
94.00	7542.0
95.00	62184.0
96.00	4276.0
97.00	142.0
103.90	351.0
104.90	153.0
105.90	365.0
113.00	105.0
115.80	276.0
116.90	484.0
117.80	297.0
118.80	449.0
127.90	261.0
128.60	137.0
128.90	127.0
129.90	255.0
130.90	115.0
137.00	156.0
140.90	663.0
141.80	106.0
142.90	852.0
144.80	297.0
147.80	195.0
154.80	202.0
157.00	154.0
170.70	163.0
171.90	883.0
173.00	765.0
173.90	52048.0
174.90	3815.0
175.90	49208.0
176.90	3251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	577.0
37.00	3038.0
38.00	2969.0
39.00	1440.0
40.00	310.0
43.00	129.0
44.00	715.0
45.00	598.0
46.00	128.0
47.00	765.0
48.00	430.0
49.00	2727.0
50.00	12693.0
51.00	3825.0
52.00	222.0
53.00	147.0
54.90	263.0
55.90	1089.0
57.00	1678.0
59.90	567.0
61.00	3557.0
62.00	3494.0
63.00	2690.0
63.90	424.0
64.90	683.0
65.90	136.0
67.00	172.0
68.00	6983.0
69.00	6737.0
70.00	543.0
72.10	512.0
73.00	3104.0
74.00	11815.0
75.00	32992.0
76.00	2967.0
76.90	534.0
78.00	259.0
78.90	2573.0
79.90	817.0
80.90	2421.0
81.90	685.0
85.90	161.0
87.00	2953.0
88.00	2613.0
91.00	314.0
92.00	1888.0
93.00	3086.0
94.00	7807.0
95.00	63680.0
96.00	4229.0
97.00	112.0
103.90	346.0
104.90	179.0
105.90	309.0
113.00	116.0
115.80	276.0
116.90	442.0
117.80	299.0
118.80	414.0
127.90	203.0
128.60	121.0
129.90	228.0
130.90	137.0
137.00	139.0
140.90	675.0
142.90	760.0
144.80	317.0
145.80	100.0
147.80	195.0
149.80	102.0
154.80	211.0
157.00	134.0
170.70	168.0
171.90	888.0
173.00	722.0
173.90	54448.0
174.90	4005.0
175.90	51752.0
176.90	3321.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	512.0
37.00	2748.0
38.00	2715.0
39.00	1363.0
40.00	324.0
40.80	107.0
43.10	118.0
43.90	724.0
45.00	547.0
46.00	102.0
47.10	684.0
48.00	402.0
49.00	2517.0
50.00	11628.0
51.00	3556.0
51.90	173.0
52.90	135.0
55.00	263.0
55.90	982.0
57.00	1517.0
59.90	488.0
61.00	3093.0
62.00	3253.0
63.00	2493.0
64.00	376.0
65.00	668.0
65.90	149.0
66.90	131.0
68.00	6453.0
69.00	6197.0
70.10	553.0
72.10	427.0
73.00	2942.0
74.00	10917.0
75.00	30032.0
76.00	2599.0
76.90	518.0
78.10	253.0
78.90	2370.0
79.90	780.0
80.90	2248.0
82.00	606.0
85.90	165.0
86.90	2750.0
88.00	2385.0
91.00	276.0
92.00	1776.0
93.00	2799.0
94.00	7432.0
95.00	59216.0
96.00	3639.0
103.90	281.0
104.90	160.0
105.90	256.0
106.90	121.0
115.90	238.0
116.80	372.0
117.70	253.0
118.80	338.0
127.90	171.0
128.70	121.0
129.80	193.0
130.80	119.0
134.70	104.0
140.90	586.0
142.90	664.0
144.80	282.0
145.70	148.0
147.80	131.0
154.80	184.0
157.00	115.0
171.10	144.0
171.80	790.0
173.00	620.0
173.90	51056.0
174.90	3766.0
175.90	49472.0
176.90	3107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284