


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035119.D
Acq On : 11 Apr 2024 08:29
Operator : SY/MD
Sample : BFB285
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB285

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Wed Apr 10 04:53:36 2024

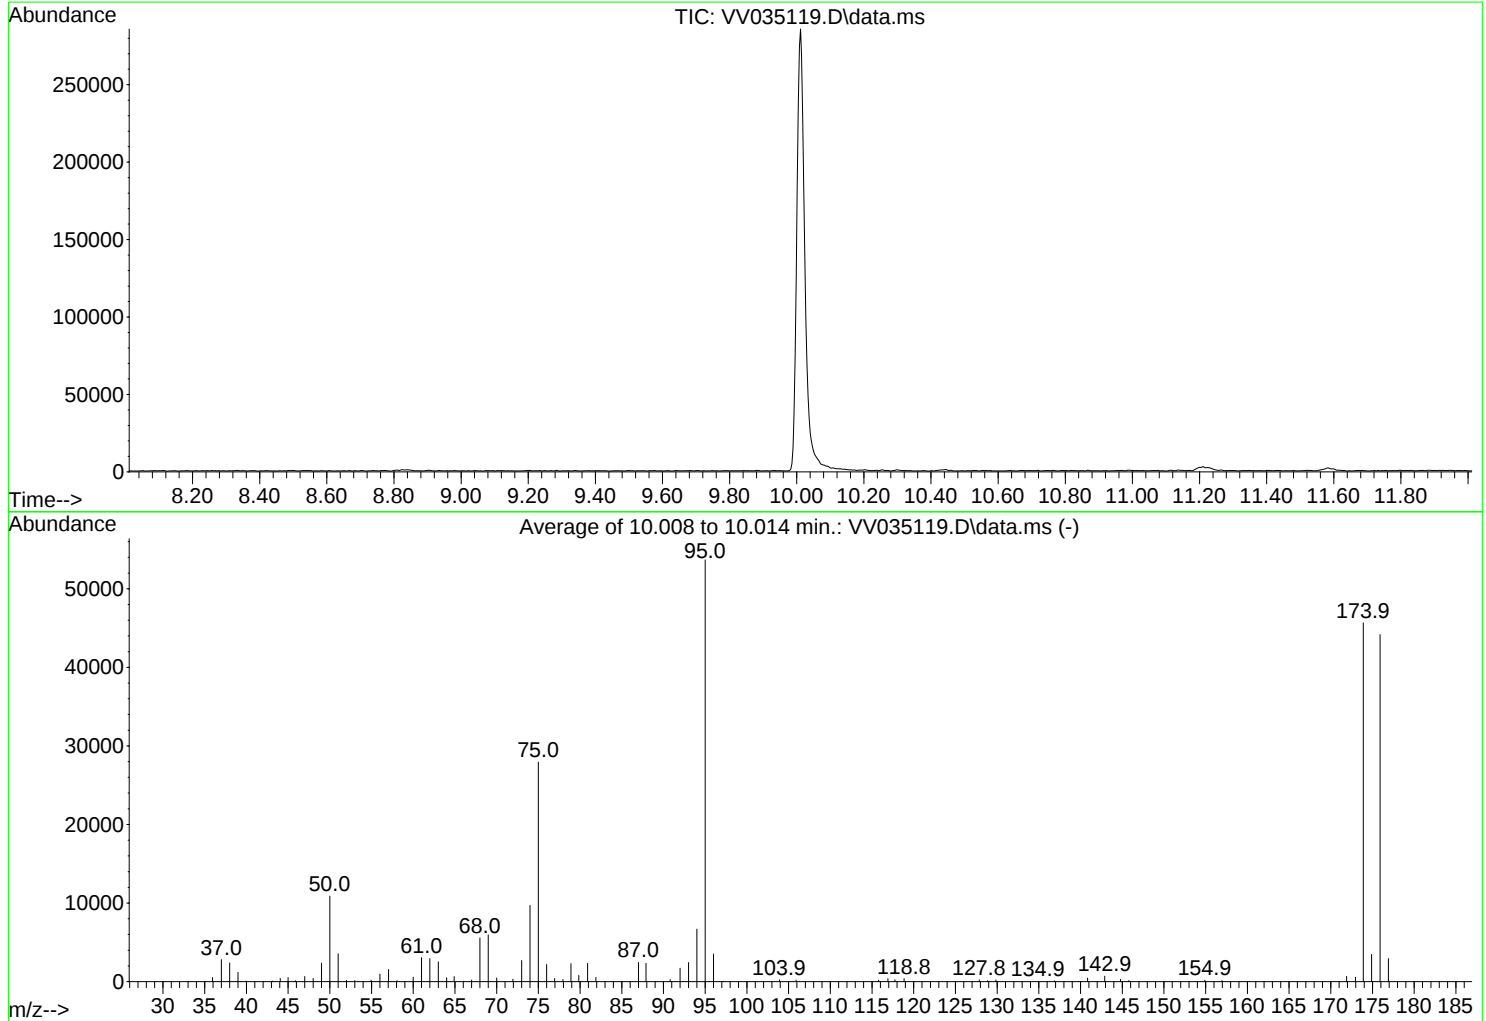

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	10904	PASS
75	95	30	80	52.0	27933	PASS
95	95	100	100	100.0	53685	PASS
96	95	5	9	6.6	3527	PASS
173	174	0.00	2	1.3	579	PASS
174	95	50	120	85.1	45667	PASS
175	174	5	9	7.6	3465	PASS
176	174	95	105	96.7	44181	PASS
177	176	5	10	6.6	2926	PASS

m/z	Abundance
39.90	215.0
44.10	423.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
36.00	518.0
37.00	2882.0
38.00	2445.0
39.00	1175.0
40.00	306.0
44.00	791.0
45.00	574.0
47.10	701.0
48.10	380.0
49.00	2352.0
50.00	11177.0
51.00	3490.0
52.00	167.0
53.00	151.0
54.90	175.0
56.00	947.0
57.00	1574.0
58.00	109.0
60.00	630.0
61.00	3044.0
62.00	2993.0
63.00	2502.0
64.00	490.0
64.90	633.0
66.00	104.0
67.10	210.0
68.00	5729.0
69.00	5950.0
70.00	454.0
71.90	295.0
73.00	2722.0
74.00	9979.0
75.00	28072.0
76.00	2211.0
76.90	378.0
77.90	282.0
78.90	2169.0
79.80	817.0
80.90	2342.0
81.90	555.0
87.00	2622.0
87.90	2284.0
90.80	286.0
92.00	1726.0
93.00	2377.0
94.00	6532.0
95.00	53752.0
96.00	3571.0
96.90	113.0
103.90	236.0
105.90	212.0
115.80	170.0
116.90	385.0
117.80	250.0
118.90	419.0
127.90	207.0
128.80	110.0
129.80	235.0
136.90	114.0
140.80	437.0
142.90	634.0
144.80	267.0
145.80	157.0
154.90	177.0
157.00	127.0
171.90	701.0
172.90	592.0
173.90	44368.0
174.90	3476.0
175.90	42728.0
176.90	2842.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
36.00	538.0
37.00	2873.0
38.00	2464.0
39.00	1240.0
40.00	295.0
43.10	102.0
44.10	839.0
45.00	568.0
45.90	156.0
47.00	653.0
48.00	416.0
49.00	2444.0
50.00	11257.0
51.00	3666.0
52.00	167.0
53.00	149.0
55.00	201.0
56.00	1010.0
57.00	1598.0
58.10	129.0
60.00	572.0
61.00	3117.0
62.00	3084.0
63.00	2599.0
64.00	516.0
64.90	657.0
66.10	109.0
67.00	205.0
68.00	5674.0
69.00	6133.0
70.00	493.0
72.00	295.0
73.00	2748.0
74.00	10061.0
75.00	28896.0
76.00	2212.0
76.90	380.0
77.90	271.0
78.90	2372.0
79.90	840.0
80.90	2433.0
81.90	539.0
87.00	2494.0
87.90	2409.0
90.80	274.0
92.00	1771.0
93.00	2509.0
94.00	7008.0
95.00	55496.0
96.00	3650.0
97.20	113.0
103.90	248.0
105.90	209.0
115.80	198.0
116.90	387.0
117.80	243.0
118.90	398.0
127.90	242.0
128.80	127.0
129.80	233.0
134.90	102.0
136.90	108.0
140.80	435.0
142.90	687.0
144.80	283.0
145.80	146.0
154.90	196.0
157.00	129.0
171.90	676.0
173.00	615.0
173.90	47344.0
174.90	3583.0
175.90	45688.0
176.90	2997.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
35.90	495.0
37.00	2684.0
38.00	2255.0
39.00	1152.0
40.00	303.0
43.10	144.0
44.00	851.0
45.00	473.0
45.90	238.0
46.90	606.0
47.90	415.0
49.00	2309.0
50.00	10279.0
51.00	3498.0
52.00	160.0
53.00	102.0
55.00	206.0
56.00	931.0
57.10	1465.0
58.10	125.0
60.00	499.0
61.00	3025.0
62.00	2708.0
63.00	2499.0
64.00	447.0
64.90	653.0
66.90	230.0
68.00	5247.0
69.00	5760.0
70.00	478.0
72.00	299.0
73.00	2569.0
74.00	9018.0
75.00	26832.0
76.00	2093.0
77.00	396.0
78.00	268.0
78.90	2292.0
79.90	752.0
80.90	2194.0
81.90	493.0
87.00	2240.0
87.90	2330.0
90.80	207.0
92.00	1650.0
93.00	2369.0
94.00	6527.0
95.00	51808.0
96.00	3361.0
103.90	204.0
105.90	217.0
115.80	207.0
116.90	349.0
117.70	234.0
118.80	353.0
127.80	247.0
128.90	113.0
129.90	210.0
134.90	105.0
136.90	111.0
140.90	499.0
142.90	752.0
144.80	279.0
145.80	109.0
154.90	194.0
156.90	113.0
171.90	640.0
173.00	531.0
173.90	45288.0
174.90	3336.0
175.90	44128.0
176.90	2938.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285