




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030504.D
 Acq On : 11 Apr 2023 19:04
 Operator : SY/MD
 Sample : 02250-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:04:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 12 05:00:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

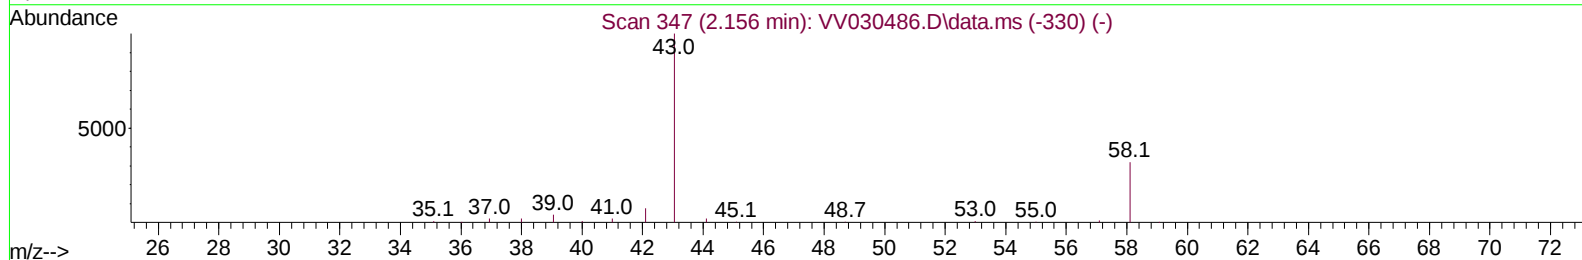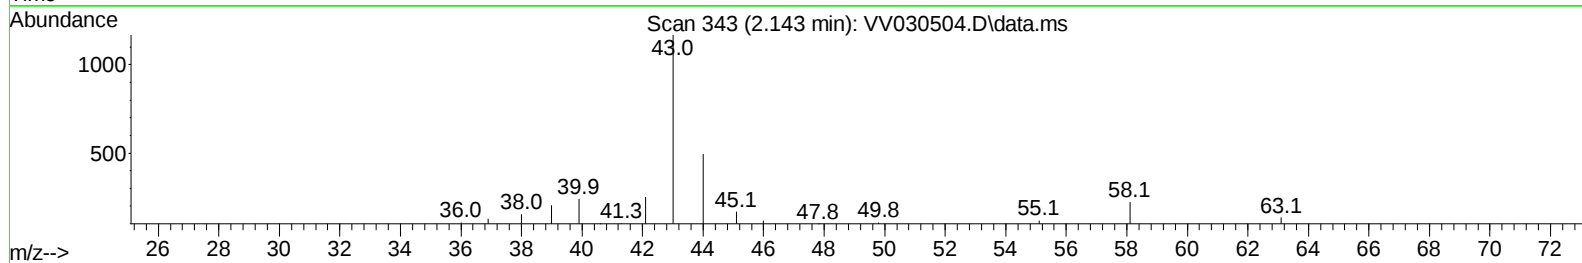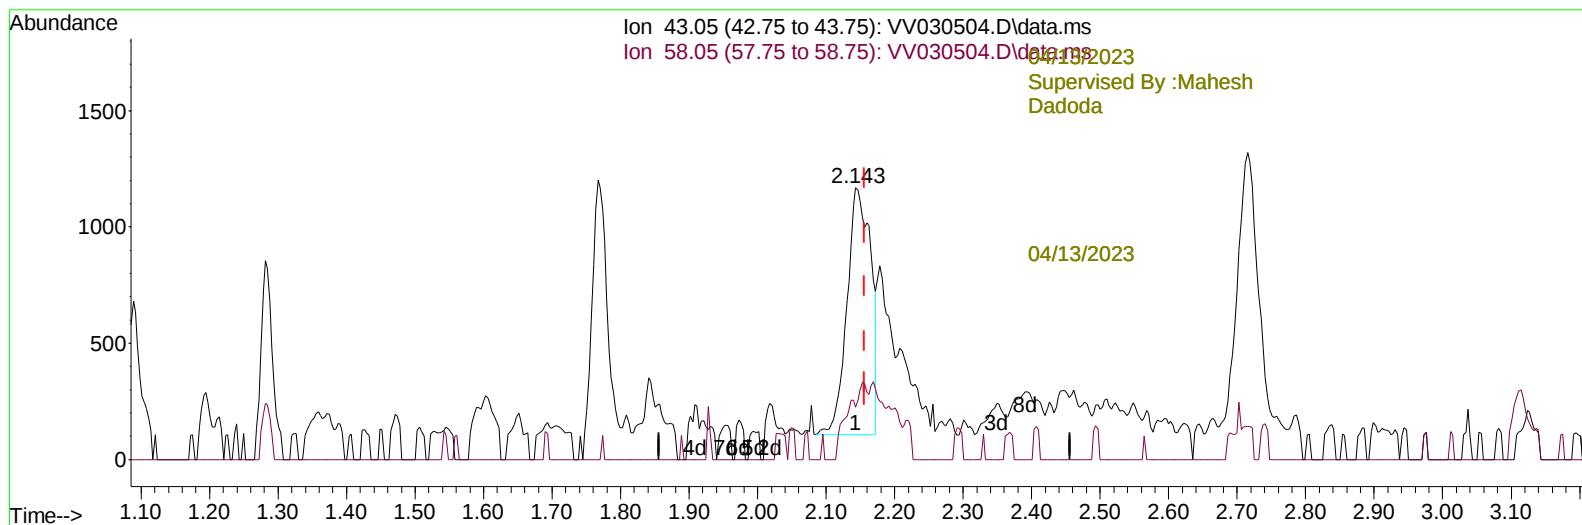

TIC: VV030504.D\data.ms

(13) Acetone (T)

2.143min (-0.013) 1.45 ug/L

response 2582

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	12.94
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030504.D
 Acq On : 11 Apr 2023 19:04
 Operator : SY/MD
 Sample : 02250-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:04:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 12 05:00:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

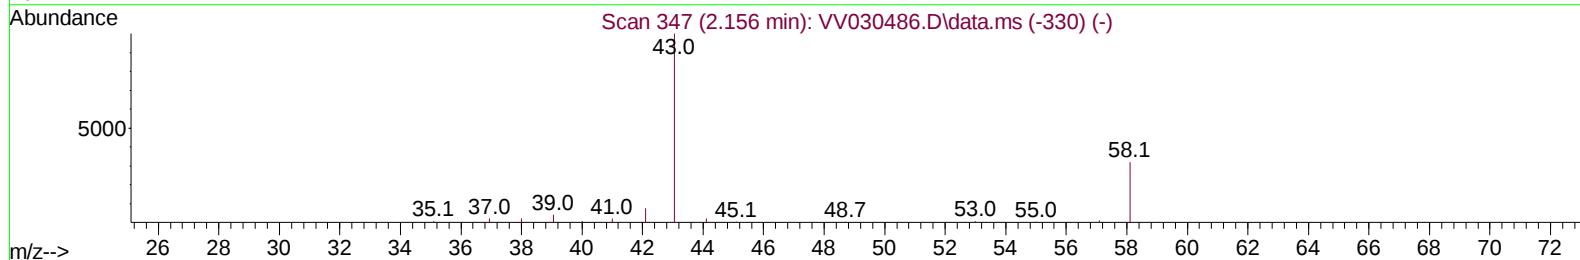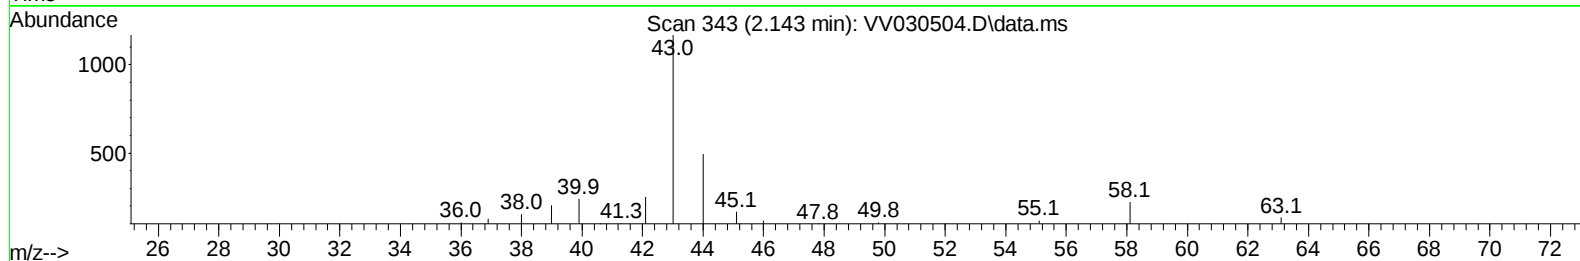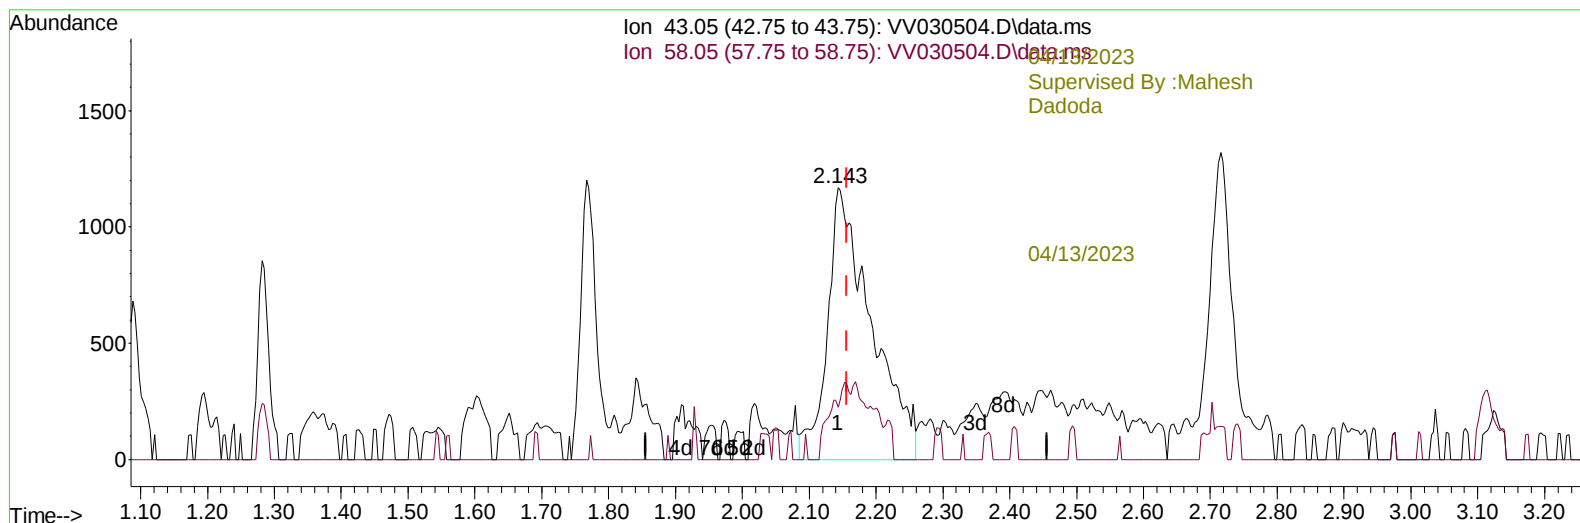

TIC: VV030504.D\data.ms

(13) Acetone (T)

2.143min (-0.013) 2.98 ug/L m

response 5308

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	6.29
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030504.D
 Acq On : 11 Apr 2023 19:04
 Operator : SY/MD
 Sample : 02250-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:04:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 12 05:00:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----04/13/2023							
Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		108974	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		108953	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		54821	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.281	65		22410	3.105	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	62.000%	
7) Chloroethane-d5	1.535	69		26712	3.814	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.200%	
11) 1,1-Dichloroethene-d2	2.066	63		51832	3.026	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.600%	
20) 2-Butanone-d5	3.822	46		83126	44.560	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.120%	
24) Chloroform-d	4.259	84		76417	4.375	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%	
26) 1,2-Dichloroethane-d4	4.953	65		38547	4.677	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%	
32) Benzene-d6	4.973	84		125277	4.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.600%	
36) 1,2-Dichloropropane-d6	5.998	67		41637	4.332	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.600%	
41) Toluene-d8	7.252	98		105157	3.730	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.600%	
43) trans-1,3-Dichloroprop...	7.564	79		13676	3.779	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.600%	
46) 2-Hexanone-d5	8.037	63		63417	43.609	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.220%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		33075	4.366	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.400%	
66) 1,2-Dichlorobenzene-d4	11.570	152		45546	4.648	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.000%	
Target Compounds							
						Qvalue	
12) 1,1-Dichloroethene	2.076	96		15871	1.743	ug/L	# 76
13) Acetone	2.143	43		5308m	2.976	ug/L	
17) Methyl tert-butyl Ether	2.715	73		11799	0.612	ug/L	98
19) 1,1-Dichloroethane	3.121	63		130571	7.021	ug/L	98
29) 1,1,1-Trichloroethane	4.529	97		11796	0.674	ug/L	97
34) Trichloroethene	5.844	95		11738	1.125	ug/L	98
47) Tetrachloroethene	7.915	164		11524	1.251	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030504.D
Acq On : 11 Apr 2023 19:04
Operator : SY/MD
Sample : 02250-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:04:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 12 05:00:18 2023
Response via : Initial Calibration

Reviewed By :Krupa
Patel

