




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030507.D
 Acq On : 11 Apr 2023 20:18
 Operator : SY/MD
 Sample : 02250-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx5

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:05:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 12 05:00:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/13/2023
 Supervised By :Mahesh Dadoda 04/13/2023

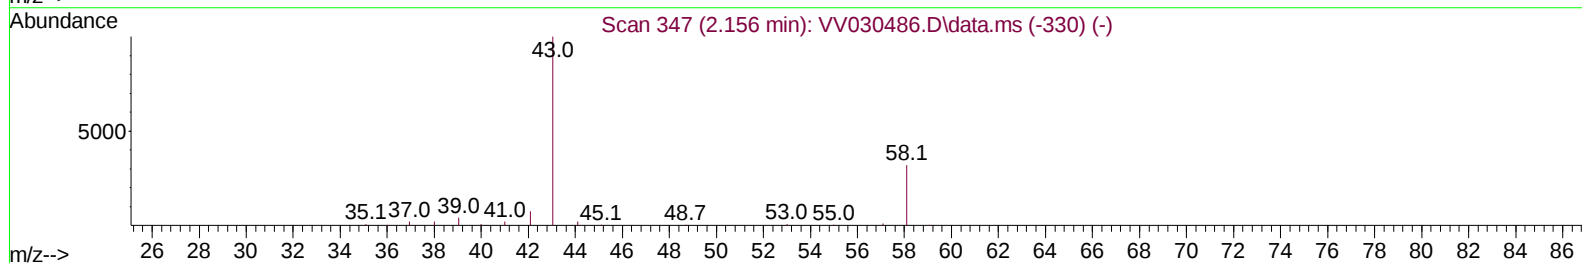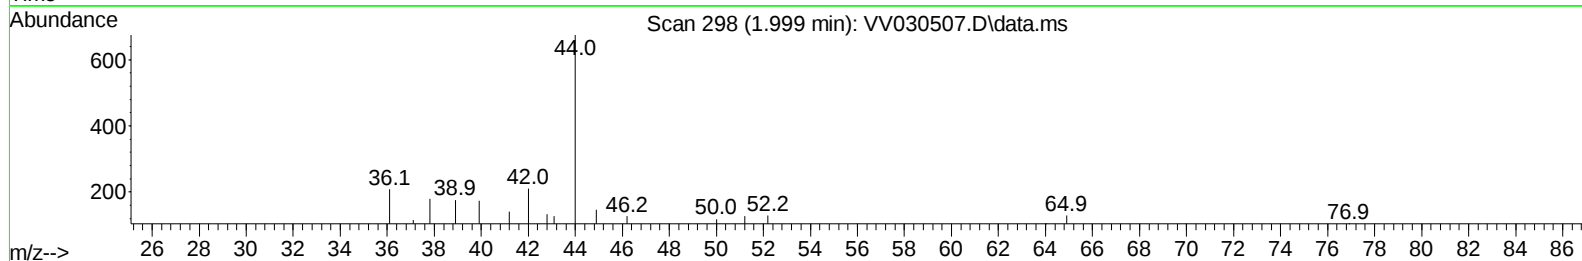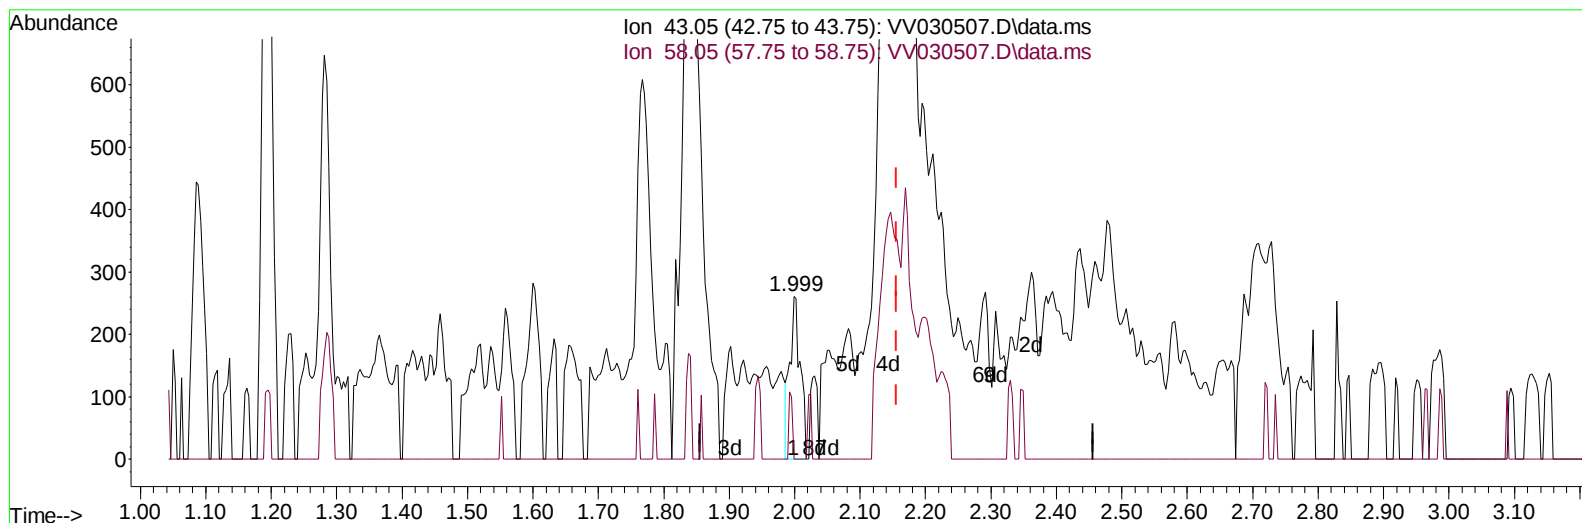

TIC: VV030507.D\data.ms

(13) Acetone (T)

1.999min (-0.158) 0.17 ug/L

response 290

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	13.79
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030507.D
 Acq On : 11 Apr 2023 20:18
 Operator : SY/MD
 Sample : 02250-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHD5

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:05:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 12 05:00:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/13/2023
 Supervised By :Mahesh Dadoda 04/13/2023

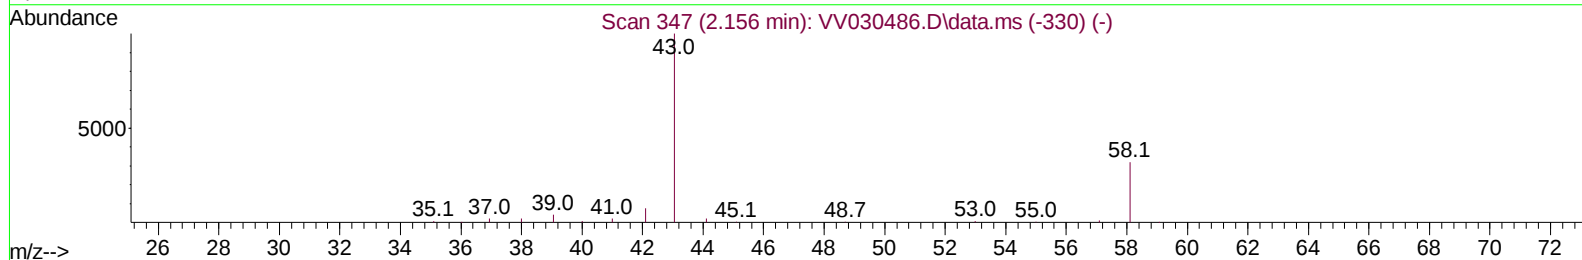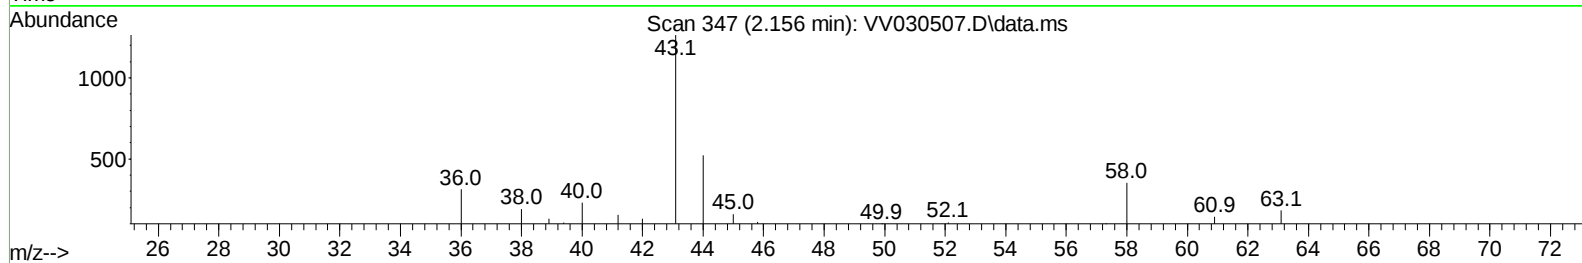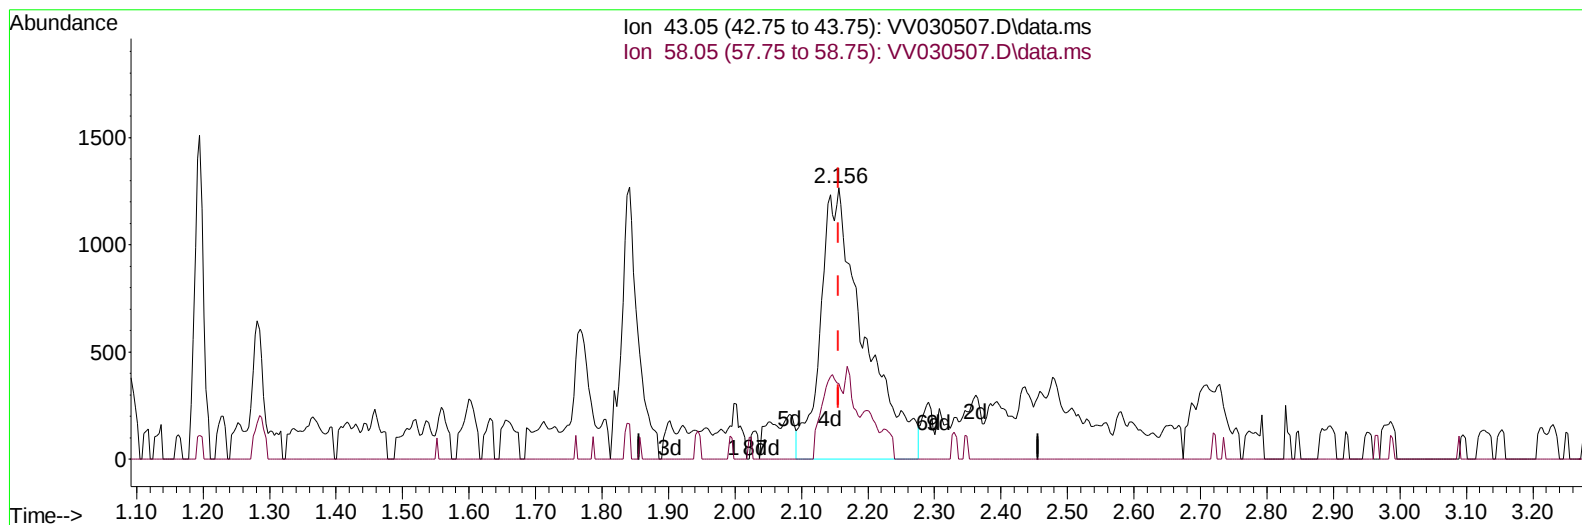

TIC: VV030507.D\data.ms

(13) Acetone (T)

2.156min (+ 0.000) 3.45 ug/L m

response 5789

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	0.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030507.D
 Acq On : 11 Apr 2023 20:18
 Operator : SY/MD
 Sample : 02250-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx5

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:05:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 12 05:00:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/13/2023
 Supervised By :Mahesh Dadoda 04/13/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	102474	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	101068	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	55524	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	21846	3.219	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	64.400%	
7) Chloroethane-d5	1.539	69	26607	4.040	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	80.800%	
11) 1,1-Dichloroethene-d2	2.066	63	61181	3.799	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	76.000%	
20) 2-Butanone-d5	3.818	46	93334	53.206	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	106.420%	
24) Chloroform-d	4.262	84	75574	4.601	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	92.000%	
26) 1,2-Dichloroethane-d4	4.957	65	38137	4.921	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	98.400%	
32) Benzene-d6	4.973	84	123465	4.335	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	86.800%	
36) 1,2-Dichloropropane-d6	5.998	67	42942	4.816	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	96.400%	
41) Toluene-d8	7.252	98	106502	4.072	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	81.400%	
43) trans-1,3-Dichloroprop...	7.561	79	13448	4.006	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	80.200%	
46) 2-Hexanone-d5	8.034	63	67464	50.011	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	100.020%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	32243	4.588	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	91.800%	
66) 1,2-Dichlorobenzene-d4	11.571	152	51104	5.150	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	103.000%	
Target Compounds						
						Qvalue
9) Trichlorofluoromethane	1.719	101	11153	0.638	ug/L	100
12) 1,1-Dichloroethene	2.076	96	33026	3.857	ug/L	90
13) Acetone	2.156	43	5789m	3.451	ug/L	
17) Methyl tert-butyl Ether	2.716	73	2643	0.146	ug/L #	73
18) trans-1,2-Dichloroethene	2.706	96	1482	0.164	ug/L	89
19) 1,1-Dichloroethane	3.121	63	103188	5.901	ug/L	98
22) cis-1,2-Dichloroethene	3.825	96	95823	10.585	ug/L	95
25) Chloroform	4.291	83	21593	1.222	ug/L	92
27) 1,2-Dichloroethane	5.060	62	2405	0.225	ug/L #	73
29) 1,1,1-Trichloroethane	4.523	97	12333	0.759	ug/L	95
34) Trichloroethene	5.841	95	245005	25.306	ug/L	98
47) Tetrachloroethene	7.915	164	131947	15.442	ug/L	97
64) 1,3-Dichlorobenzene	11.130	146	1855	0.091	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030507.D
Acq On : 11 Apr 2023 20:18
Operator : SY/MD
Sample : 02250-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx5

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:05:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 12 05:00:18 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/13/2023
Supervised By :Mahesh Dadoda 04/13/2023

