

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041123\
 Data File : VW030487.D
 Acq On : 11 Apr 2023 12:10
 Operator : SY/MD
 Sample : VW0411WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK326

Quant Time: Apr 12 05:01:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 12 05:00:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	114523	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	112641	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	54777	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	30308	3.996	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.536	69	28970	3.936	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.800%
11) 1,1-Dichloroethene-d2	2.063	63	54123	3.007	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.200%
20) 2-Butanone-d5	3.828	46	60083	30.647	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	61.300%
24) Chloroform-d	4.259	84	74425	4.054	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.000%
26) 1,2-Dichloroethane-d4	4.953	65	35421	4.090	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.800%
32) Benzene-d6	4.966	84	130895	4.124	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.400%
36) 1,2-Dichloropropane-d6	5.995	67	40822	4.108	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.200%
41) Toluene-d8	7.249	98	113668	3.900	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.000%
43) trans-1,3-Dichloroprop...	7.561	79	13660	3.651	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.000%
46) 2-Hexanone-d5	8.037	63	47589	31.653	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	63.300%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	28451	3.633	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	72.600%
66) 1,2-Dichlorobenzene-d4	11.570	152	42786	4.370	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.400%
Target Compounds						
16) Methylene chloride	2.452	84	8835	0.781	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030487.D
Acq On : 11 Apr 2023 12:10
Operator : SY/MD
Sample : VV0411WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK326

Quant Time: Apr 12 05:01:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 12 05:00:18 2023
Response via : Initial Calibration

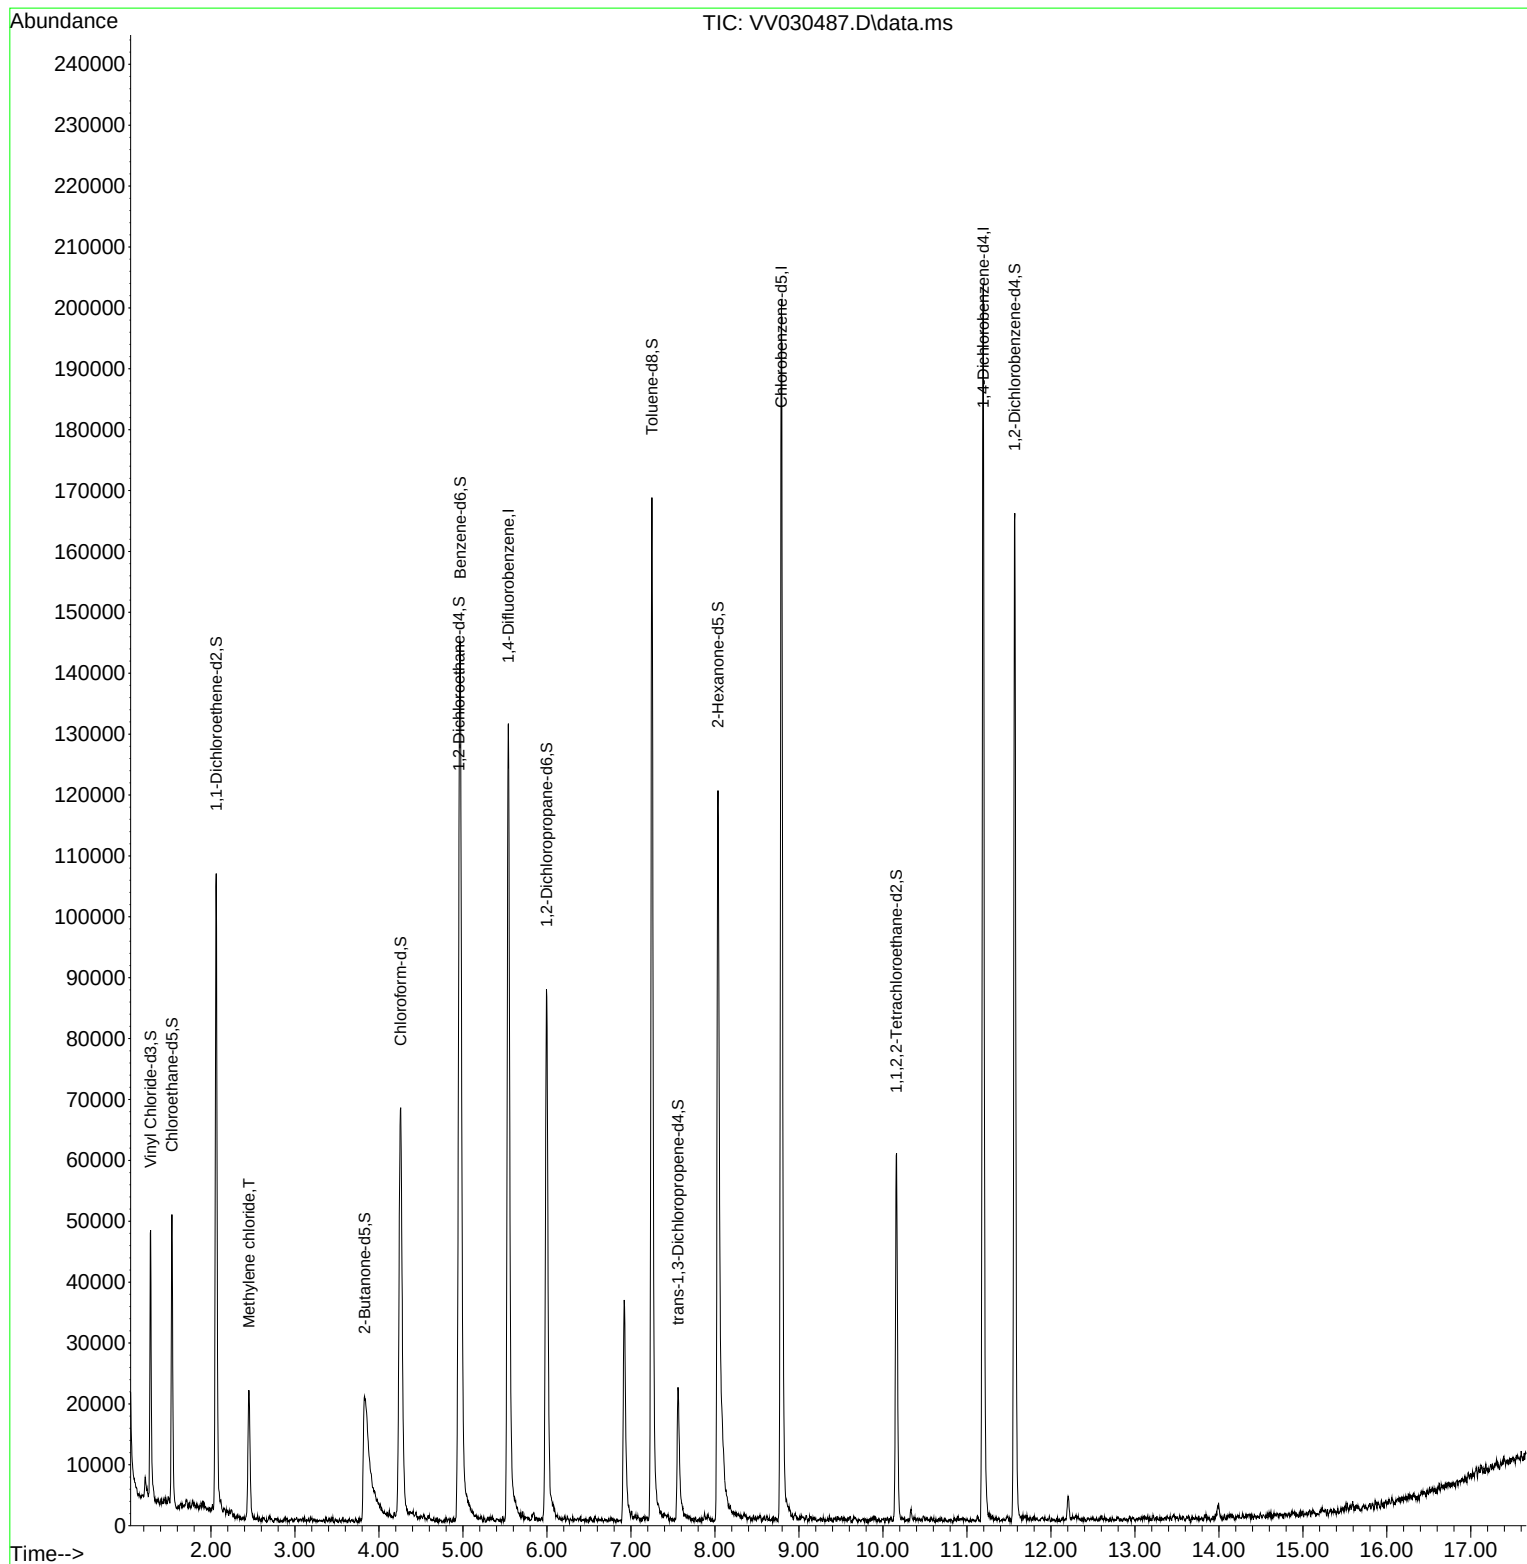

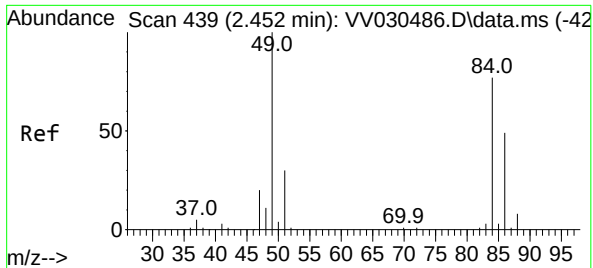

#16
Methylene chloride
Concen: 0.781 ug/L
RT: 2.452 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV030487.D
Acq: 11 Apr 2023 12:10

Instrument :
MSVOA_V
ClientSampleId :
VBLK326

Tgt Ion:	84	Resp:	8835
Ion	Ratio	Lower	Upper
84	100		
86	63.4	44.0	81.6
49	128.4	90.6	168.3

