

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041123\
 Data File : VW030503.D
 Acq On : 11 Apr 2023 18:39
 Operator : SY/MD
 Sample : 02250-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY2

Quant Time: Apr 12 05:04:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 12 05:00:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	104770	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	105629	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	51435	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	23541	3.393	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.800%
7) Chloroethane-d5	1.539	69	27652	4.106	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.200%
11) 1,1-Dichloroethene-d2	2.063	63	45433	2.759	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.200%#
20) 2-Butanone-d5	3.822	46	85129	47.465	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.920%
24) Chloroform-d	4.259	84	76680	4.566	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
26) 1,2-Dichloroethane-d4	4.957	65	39366	4.968	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	4.969	84	128773	4.326	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%
36) 1,2-Dichloropropane-d6	5.998	67	42624	4.574	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.400%
41) Toluene-d8	7.252	98	107182	3.921	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%
43) trans-1,3-Dichloroprop...	7.564	79	13455	3.835	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.600%
46) 2-Hexanone-d5	8.037	63	64279	45.592	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.180%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	33291	4.533	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.600%
66) 1,2-Dichlorobenzene-d4	11.570	152	46106	5.015	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.400%
Target Compounds					Qvalue	
13) Acetone	2.153	43	3794	2.212	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030503.D
Acq On : 11 Apr 2023 18:39
Operator : SY/MD
Sample : 02250-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY2

Quant Time: Apr 12 05:04:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 12 05:00:18 2023
Response via : Initial Calibration

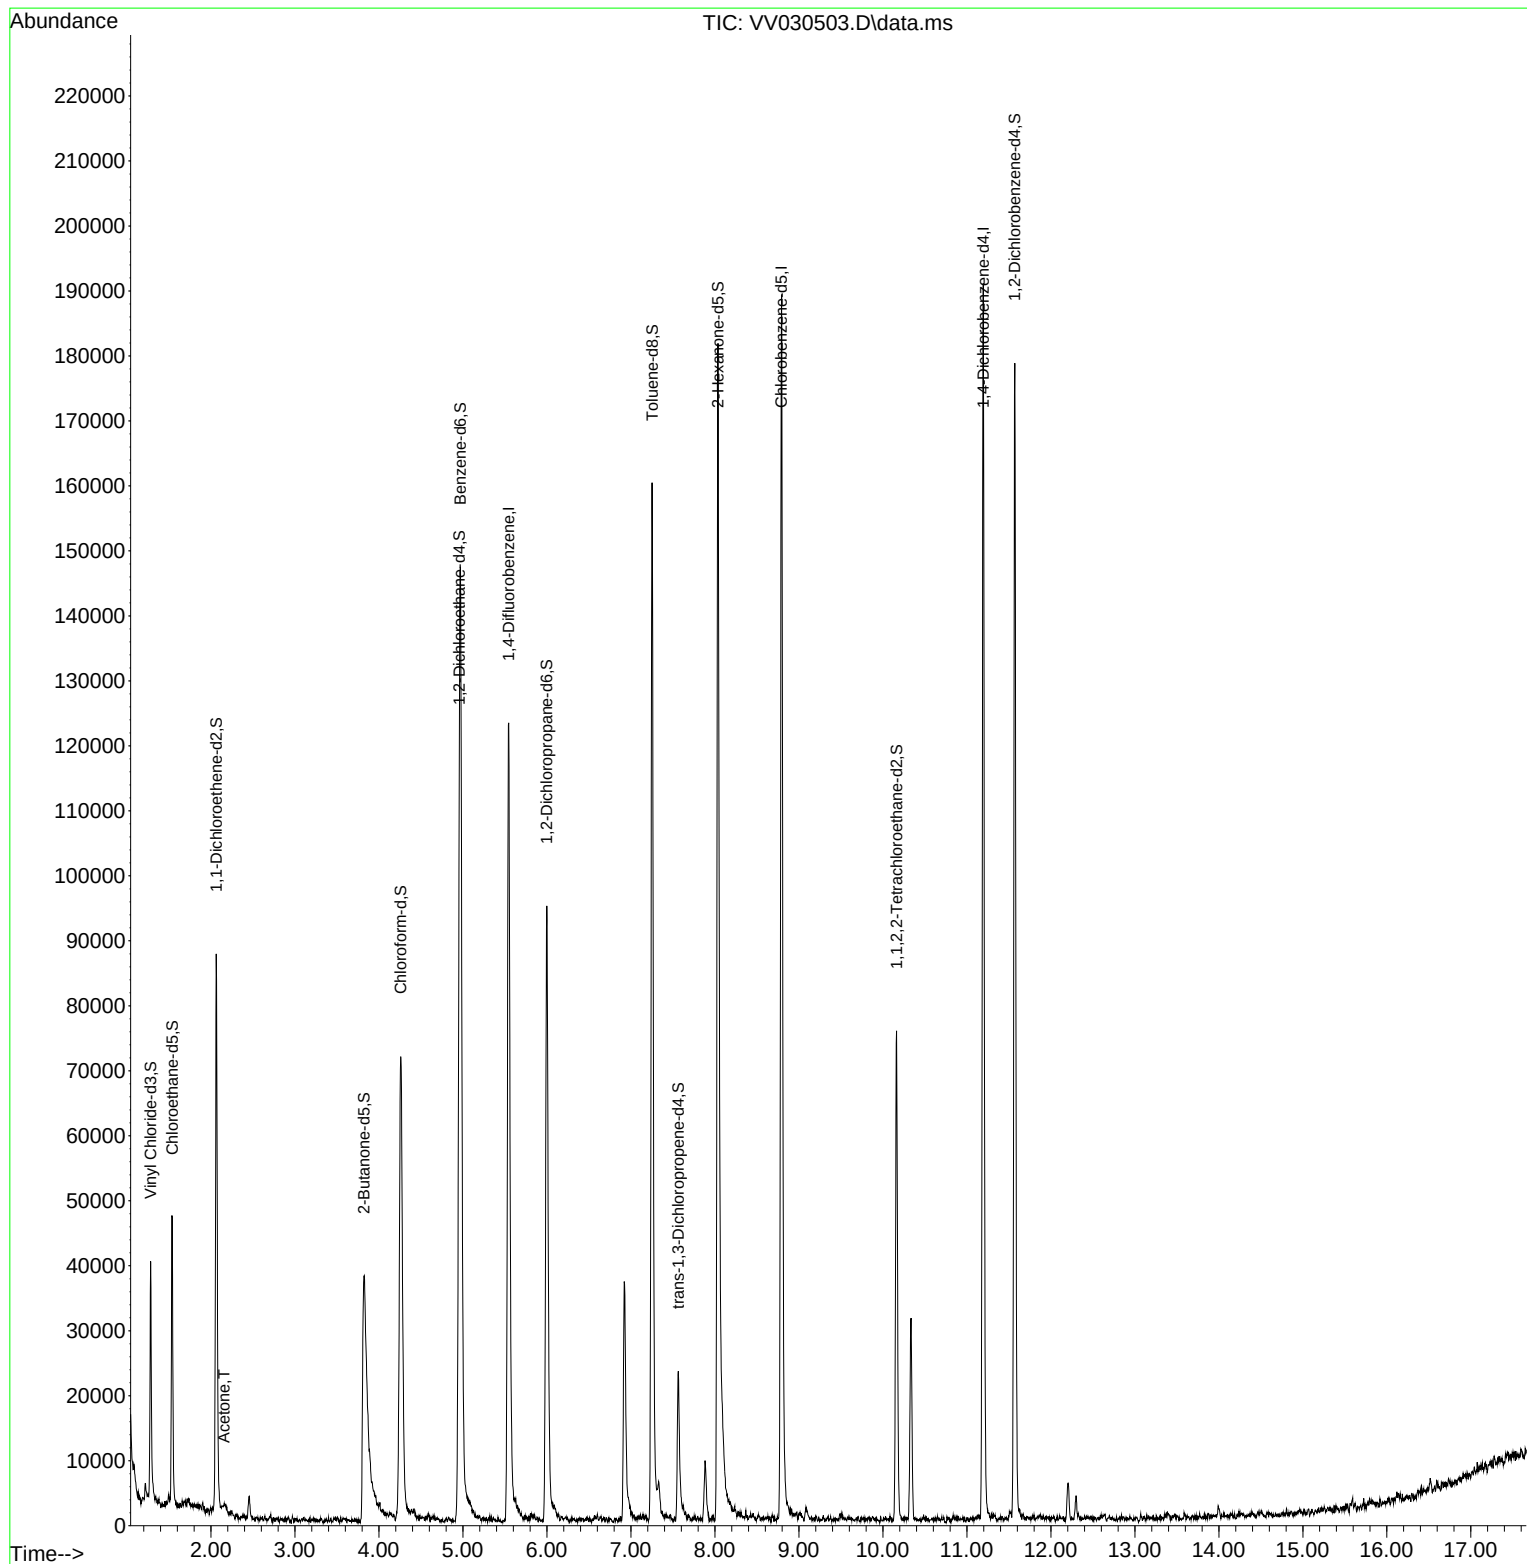

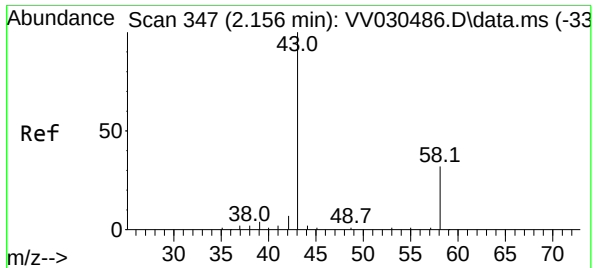

#13
 Acetone
 Concen: 2.212 ug/L
 RT: 2.153 min Scan# 34
 Delta R.T. -0.003 min
 Lab File: VV030503.D
 Acq: 11 Apr 2023 18:39

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY2

Tgt Ion: 43	Resp: 3794
Ion Ratio	Lower Upper
43	100
58	14.6 0.0 40.8

