

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030487.D
 Acq On : 11 Apr 2023 12:10
 Operator : SY/MD
 Sample : VV0411WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK326

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	61	rBV3	3179	3814	1.00%	0.122%
2	1.282	68	75	92	rVB	44463	53050	13.94%	1.702%
3	1.536	146	154	171	rVB	48312	59832	15.72%	1.920%
4	2.063	308	318	332	rBV	104358	154739	40.65%	4.965%
5	2.452	424	439	456	rBV2	21342	38779	10.19%	1.244%
6	3.828	857	867	869	rBV	20204	28685	7.54%	0.920%
7	4.259	986	1001	1021	rBV2	66289	172467	45.31%	5.534%
8	4.966	1204	1221	1251	rBV2	144386	380653	100.00%	12.215%
9	5.542	1386	1400	1422	rBV	130978	281894	74.06%	9.046%
10	5.995	1527	1541	1563	rBV2	87227	190280	49.99%	6.106%
11	6.921	1818	1829	1844	rBV	36543	73514	19.31%	2.359%
12	7.249	1919	1931	1952	rBV	167958	306313	80.47%	9.829%
13	7.561	2019	2028	2049	rBV	21727	44919	11.80%	1.441%
14	8.037	2163	2176	2205	rBV	120018	277188	72.82%	8.895%
15	8.792	2398	2411	2428	rBV	200757	344619	90.53%	11.058%
16	10.162	2822	2837	2854	rBV	60516	101518	26.67%	3.258%
17	11.194	3147	3158	3176	rBV	203378	328132	86.20%	10.529%
18	11.571	3262	3275	3292	rBV	165664	270104	70.96%	8.667%
19	12.204	3465	3472	3480	rBV3	3823	5855	1.54%	0.188%




Sum of corrected areas: 3116355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030487.D
Acq On : 11 Apr 2023 12:10
Operator : SY/MD
Sample : VV0411WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

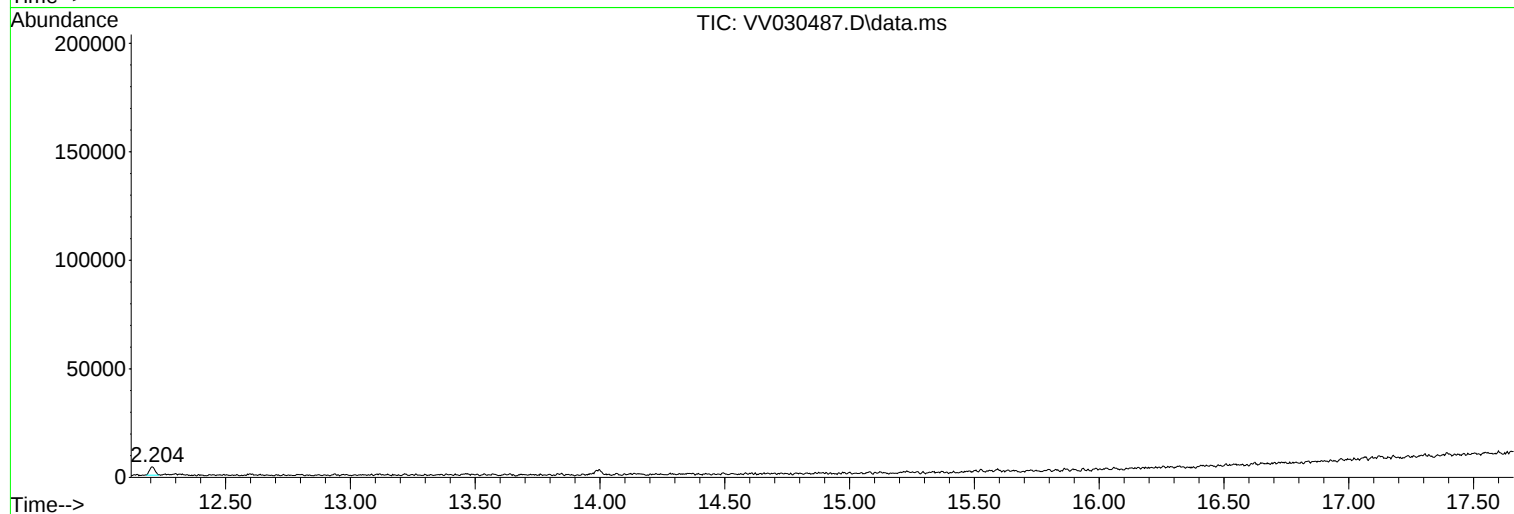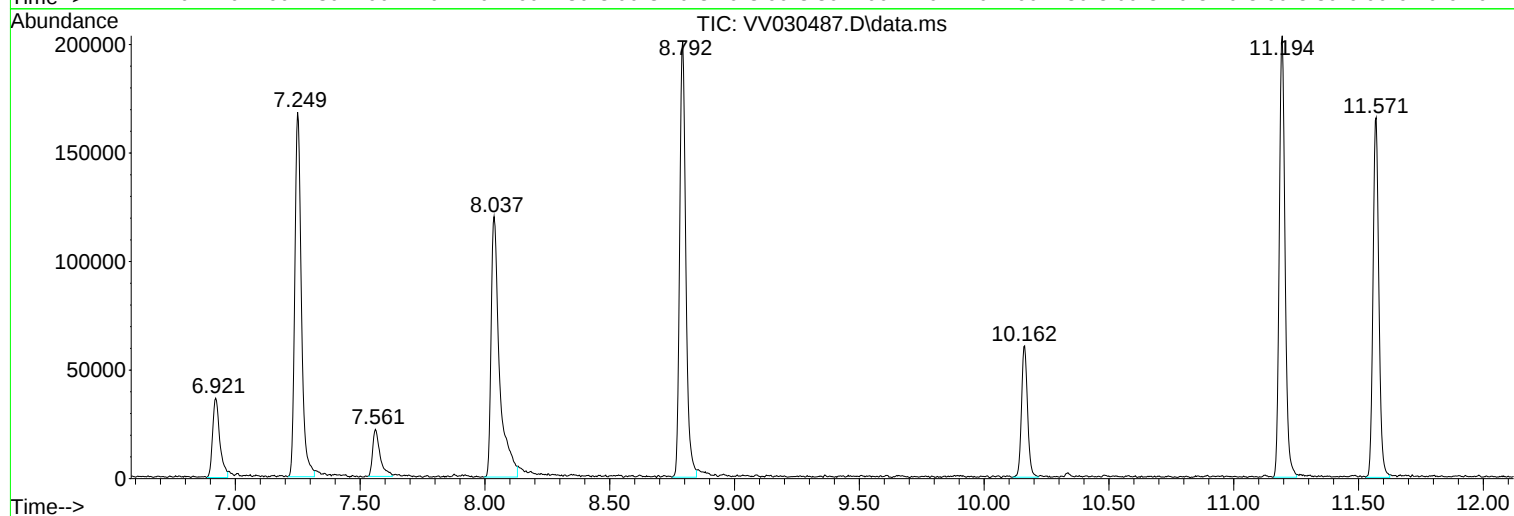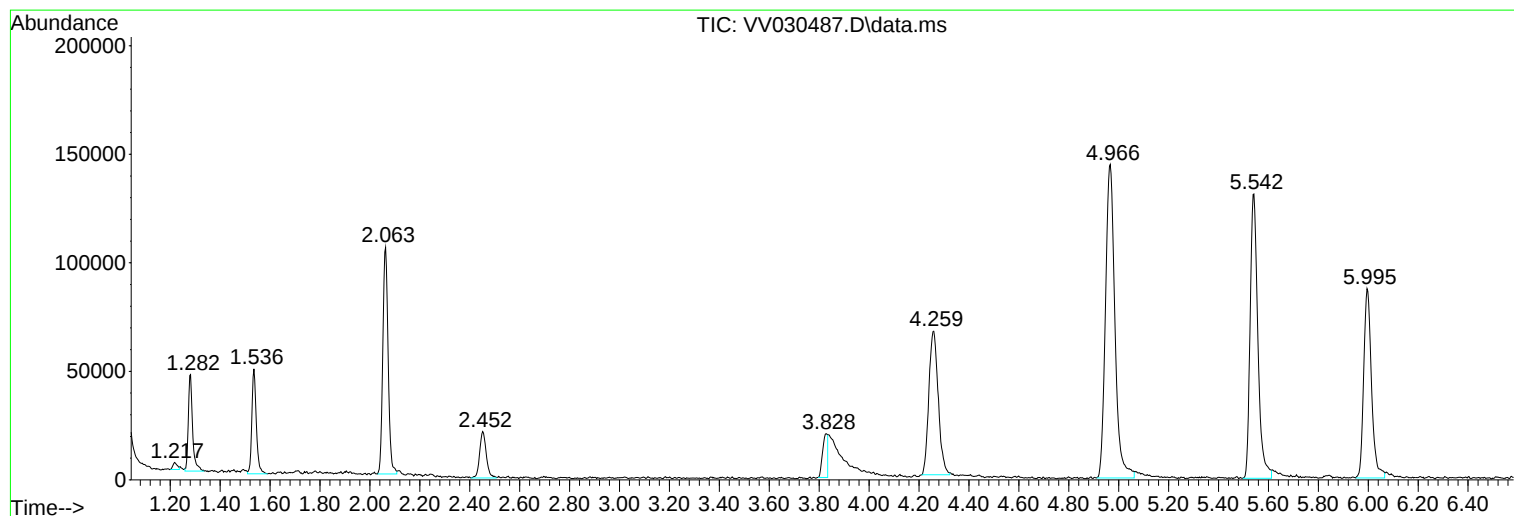

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030487.D
Acq On : 11 Apr 2023 12:10
Operator : SY/MD
Sample : VV0411WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030487.D
Acq On : 11 Apr 2023 12:10
Operator : SY/MD
Sample : VV0411WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc