

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030488.D
 Acq On : 11 Apr 2023 12:38
 Operator : SY/MD
 Sample : 02225-13DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	41143	45507	10.96%	1.169%
2	1.536	146	154	168	rVB	51060	60113	14.47%	1.544%
3	2.069	308	320	335	rBV3	149821	254544	61.28%	6.537%
4	2.452	429	439	457	rVB	40786	71811	17.29%	1.844%
5	3.831	856	868	902	rBV2	27334	128366	30.91%	3.297%
6	4.259	981	1001	1026	rBV	76631	201226	48.45%	5.168%
7	4.519	1064	1082	1104	rBV	137708	360240	86.73%	9.252%
8	4.966	1202	1221	1246	rBV3	158821	415349	100.00%	10.667%
9	5.542	1387	1400	1426	rBV2	126356	270180	65.05%	6.939%
10	5.838	1484	1492	1504	rBV2	3475	7441	1.79%	0.191%
11	5.998	1524	1542	1563	rBV2	98356	213298	51.35%	5.478%
12	6.921	1818	1829	1845	rBV2	38731	76059	18.31%	1.953%
13	7.252	1916	1932	1956	rBV	173100	320313	77.12%	8.226%
14	7.561	2018	2028	2045	rBV	24338	48752	11.74%	1.252%
15	8.037	2165	2176	2210	rBV	164283	364352	87.72%	9.357%
16	8.793	2398	2411	2437	rBV	191137	329770	79.40%	8.469%
17	10.162	2826	2837	2855	rBV	72943	122727	29.55%	3.152%
18	11.194	3143	3158	3178	rBV	190206	304919	73.41%	7.831%
19	11.571	3262	3275	3294	rBV	180454	292417	70.40%	7.510%
20	12.204	3464	3472	3484	rVB5	3307	6413	1.54%	0.165%




Sum of corrected areas: 3893797

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030488.D
Acq On : 11 Apr 2023 12:38
Operator : SY/MD
Sample : 02225-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

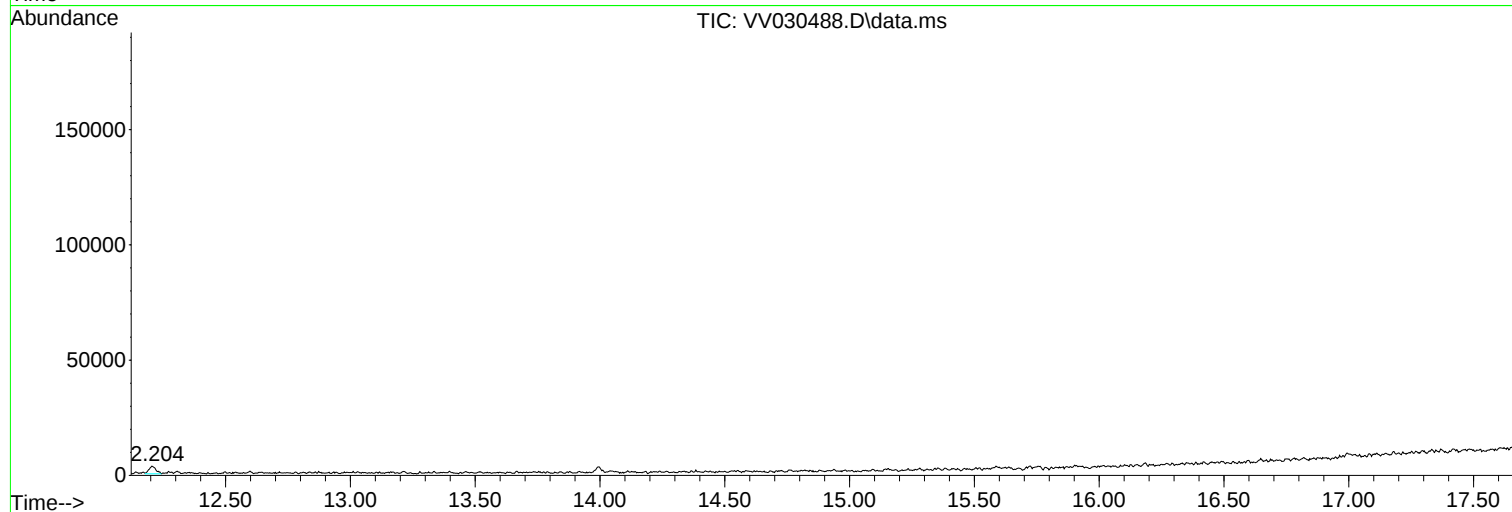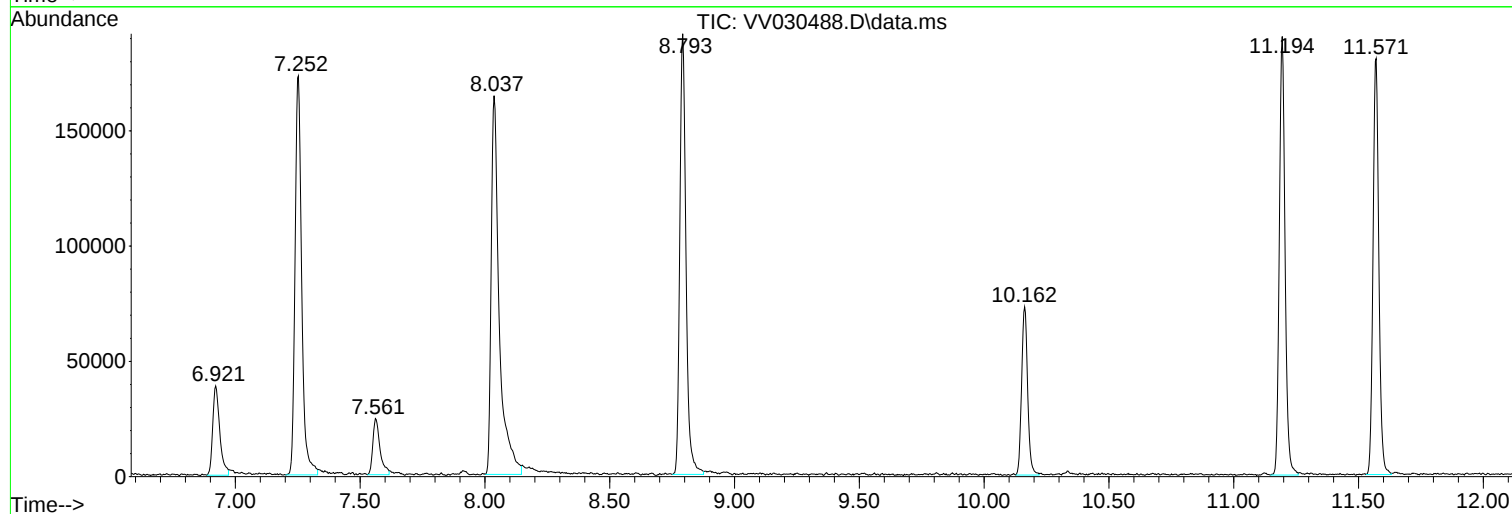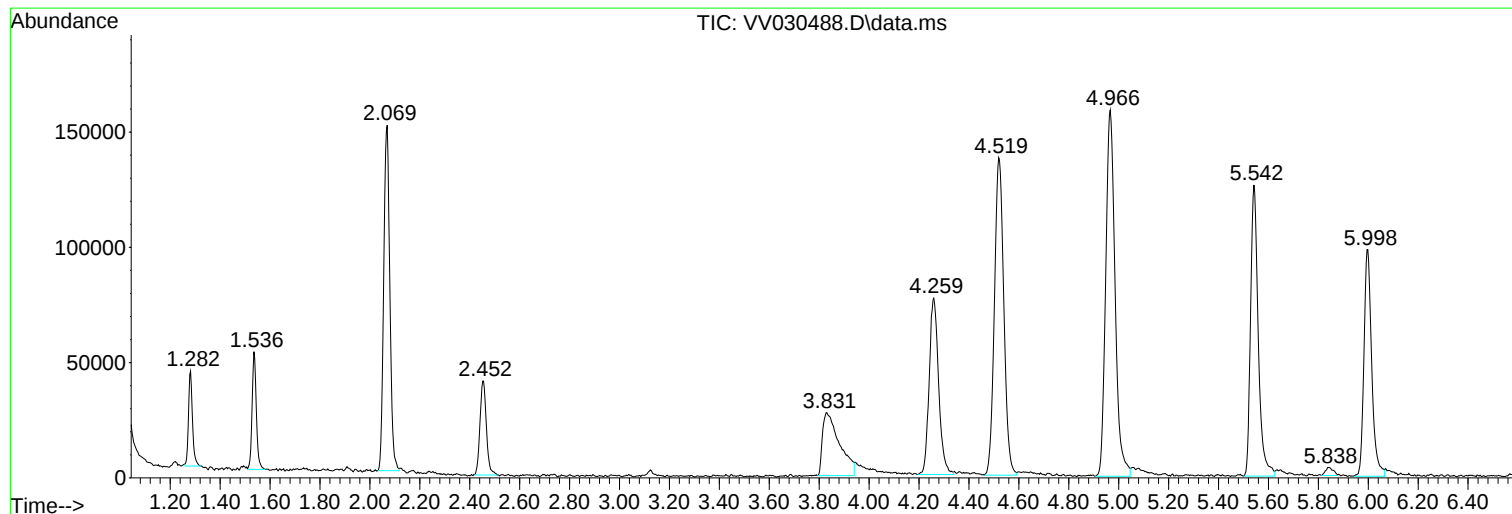

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030488.D
Acq On : 11 Apr 2023 12:38
Operator : SY/MD
Sample : 02225-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030488.D
Acq On : 11 Apr 2023 12:38
Operator : SY/MD
Sample : 02225-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc