

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030489.D
 Acq On : 11 Apr 2023 13:00
 Operator : SY/MD
 Sample : 02194-15DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rVB	38780	46400	11.55%	1.126%
2	1.535	147	154	169	rVB	47230	57381	14.28%	1.392%
3	2.063	309	318	330	rBV2	92400	137681	34.27%	3.340%
4	2.455	427	440	458	rBV	51169	89784	22.35%	2.178%
5	2.715	508	521	531	rBV7	4419	11480	2.86%	0.278%
6	3.828	849	867	897	rBV2	103272	324626	80.81%	7.874%
7	4.262	987	1002	1026	rVB2	70340	179043	44.57%	4.343%
8	4.969	1204	1222	1242	rBV3	147207	379673	94.51%	9.210%
9	5.545	1386	1401	1425	rBV2	128223	276698	68.88%	6.712%
10	5.844	1481	1494	1515	rBV	104495	217176	54.06%	5.268%
11	5.998	1530	1542	1569	rVB2	91393	194505	48.42%	4.718%
12	6.924	1820	1830	1850	rBV	35648	71740	17.86%	1.740%
13	7.252	1917	1932	1954	rBV	157176	295175	73.48%	7.160%
14	7.564	2020	2029	2049	rBV2	23037	45431	11.31%	1.102%
15	7.915	2123	2138	2158	rBV	229940	401735	100.00%	9.745%
16	8.040	2166	2177	2210	rBV	151434	350234	87.18%	8.496%
17	8.792	2399	2411	2429	rBV	198318	336530	83.77%	8.163%
18	10.162	2822	2837	2850	rBV2	69258	116187	28.92%	2.818%
19	11.194	3147	3158	3177	rBV	197478	315639	78.57%	7.656%
20	11.570	3264	3275	3292	rBV	164342	270530	67.34%	6.562%
21	13.992	4022	4028	4034	rBV3	3492	4876	1.21%	0.118%




Sum of corrected areas: 4122524

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030489.D
Acq On : 11 Apr 2023 13:00
Operator : SY/MD
Sample : 02194-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

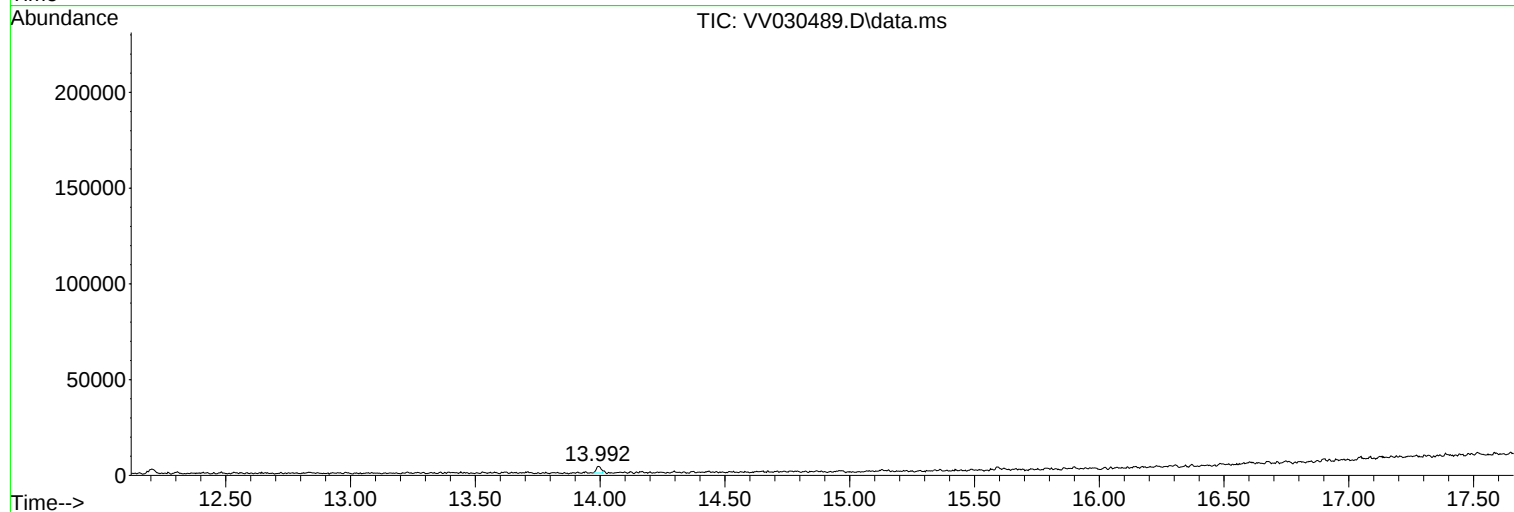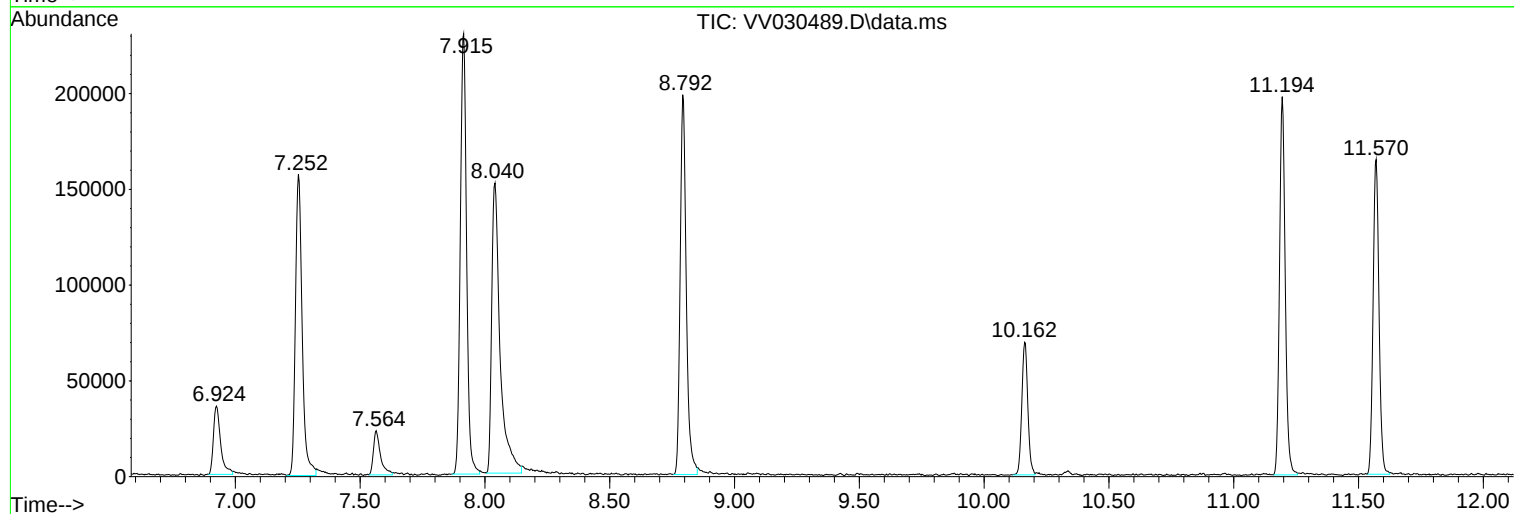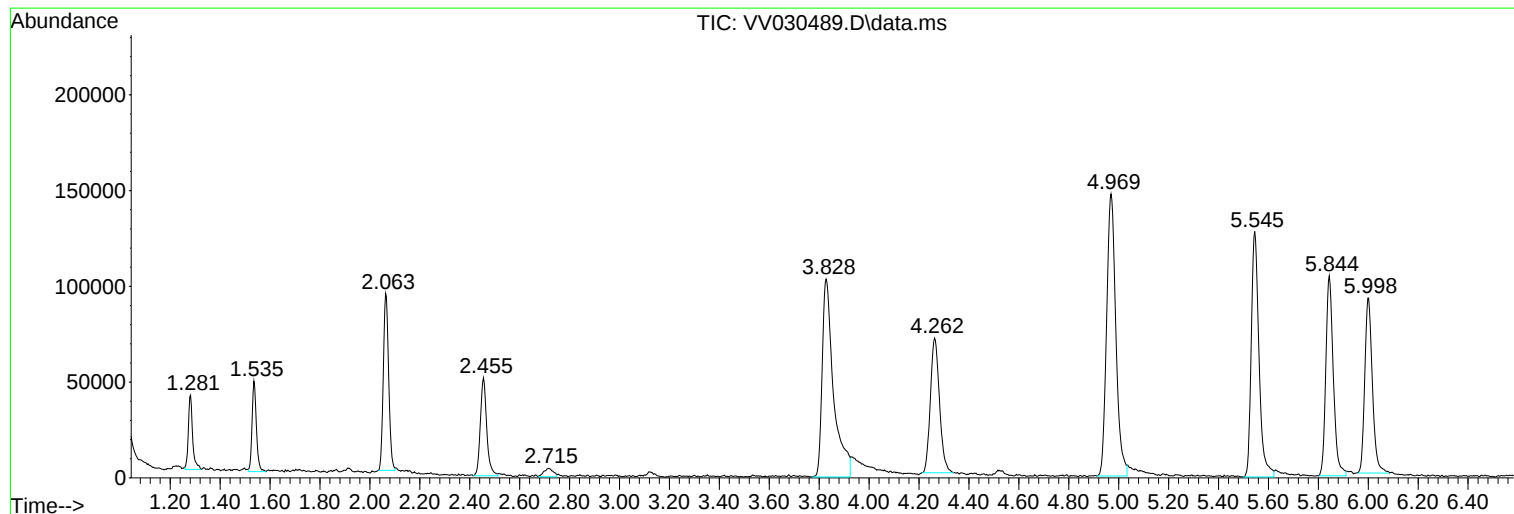

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030489.D
Acq On : 11 Apr 2023 13:00
Operator : SY/MD
Sample : 02194-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030489.D
Acq On : 11 Apr 2023 13:00
Operator : SY/MD
Sample : 02194-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------