

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030490.D
 Acq On : 11 Apr 2023 13:25
 Operator : SY/MD
 Sample : 02250-14DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	40563	45037	7.87%	1.050%
2	1.539	146	155	168	rVV	46207	56552	9.89%	1.319%
3	2.066	309	319	336	rBV2	90863	139515	24.39%	3.253%
4	2.455	429	440	454	rBV2	28949	51331	8.97%	1.197%
5	3.822	852	865	899	rBV3	72039	241449	42.21%	5.630%
6	4.262	982	1002	1021	rBV2	76328	196351	34.33%	4.579%
7	4.969	1205	1222	1250	rBV2	147874	416264	72.78%	9.707%
8	5.545	1385	1401	1419	rBV	122823	259882	45.44%	6.060%
9	5.841	1480	1493	1515	rBV2	125253	264530	46.25%	6.168%
10	5.998	1527	1542	1563	rBV2	94360	203932	35.65%	4.755%
11	6.921	1817	1829	1845	rBV	37581	74253	12.98%	1.731%
12	7.252	1920	1932	1955	rBV	163728	301859	52.77%	7.039%
13	7.564	2018	2029	2044	rBV2	23760	46380	8.11%	1.082%
14	7.911	2119	2137	2159	rBV	334959	571979	100.00%	13.338%
15	8.037	2163	2176	2207	rBV	177214	365337	63.87%	8.519%
16	8.792	2399	2411	2429	rBV	193725	329431	57.59%	7.682%
17	10.162	2826	2837	2849	rBV	71466	116508	20.37%	2.717%
18	10.333	2881	2890	2901	rVB2	6272	11041	1.93%	0.257%
19	11.194	3146	3158	3172	rBV	194498	308520	53.94%	7.194%
20	11.570	3262	3275	3288	rBV	175078	281324	49.18%	6.560%
21	12.204	3462	3472	3482	rBV3	4252	6989	1.22%	0.163%




Sum of corrected areas: 4288464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030490.D
Acq On : 11 Apr 2023 13:25
Operator : SY/MD
Sample : 02250-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

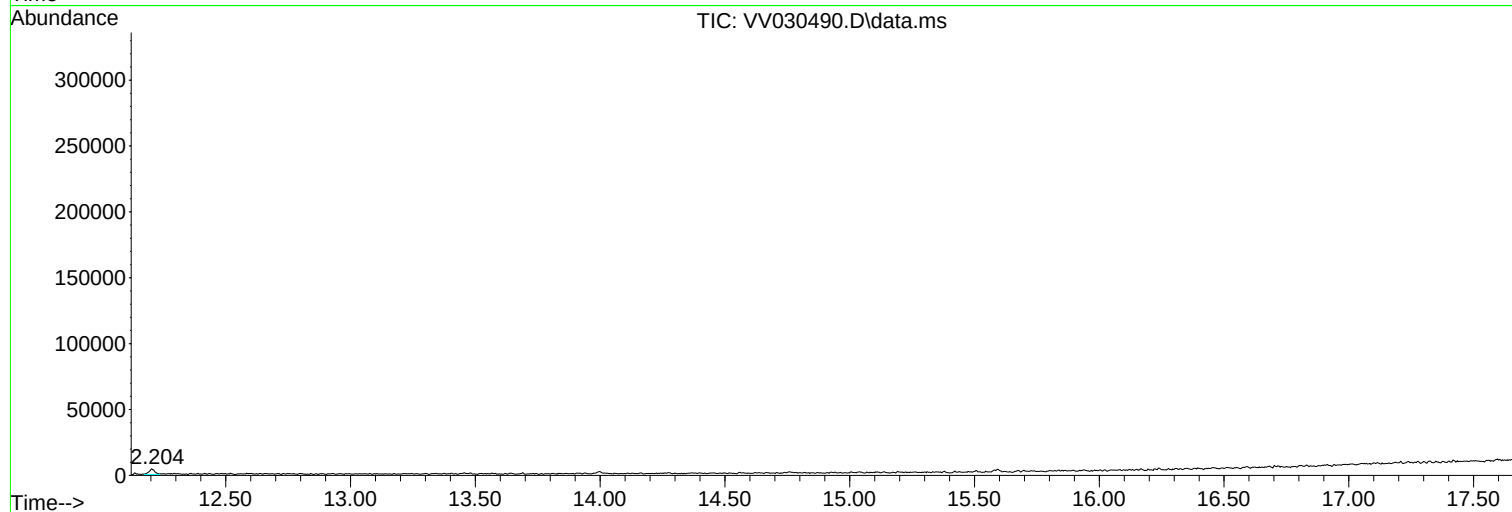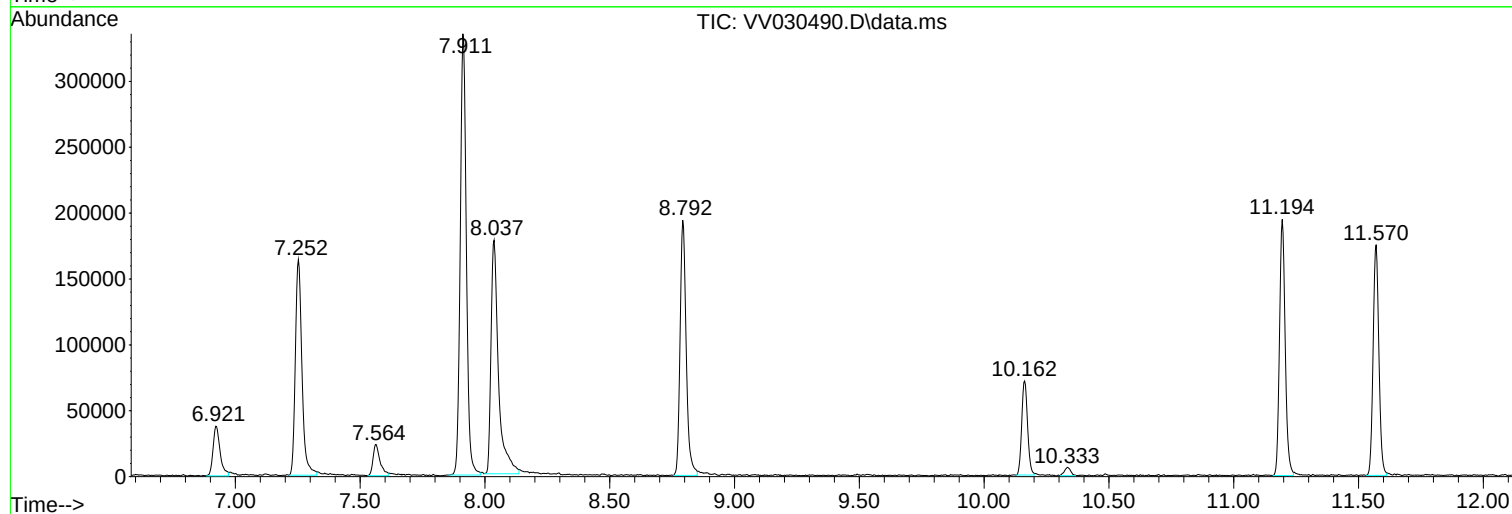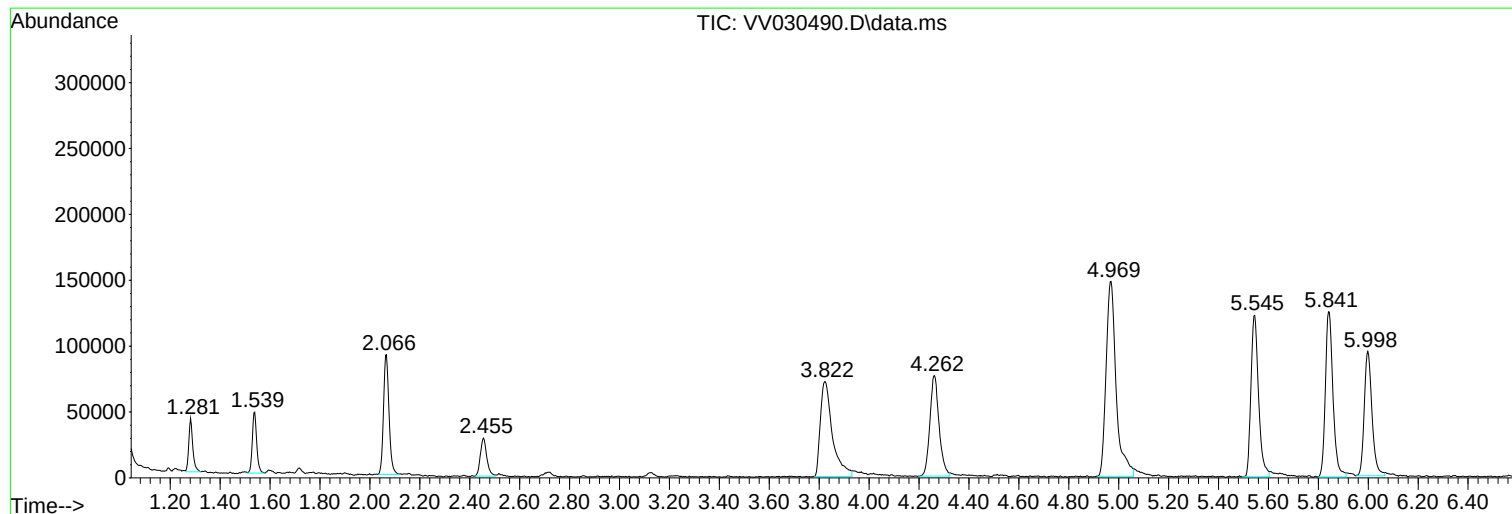

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030490.D
Acq On : 11 Apr 2023 13:25
Operator : SY/MD
Sample : 02250-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030490.D
Acq On : 11 Apr 2023 13:25
Operator : SY/MD
Sample : 02250-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------