

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030494.D
 Acq On : 11 Apr 2023 14:58
 Operator : SY/MD
 Sample : 02250-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	36467	43276	11.27%	1.273%
2	1.539	147	155	170	rVB	45407	57521	14.98%	1.693%
3	2.066	307	319	329	rBV	86322	125398	32.65%	3.690%
4	2.458	429	441	450	rBV4	3921	7689	2.00%	0.226%
5	3.815	852	863	901	rBV	40335	150405	39.16%	4.426%
6	4.262	985	1002	1026	rBV2	71587	191270	49.81%	5.628%
7	4.969	1204	1222	1249	rBV2	145110	384030	100.00%	11.301%
8	5.542	1385	1400	1421	rBV	121327	259082	67.46%	7.624%
9	5.998	1529	1542	1558	rBV2	92793	195677	50.95%	5.758%
10	6.921	1819	1829	1852	rBV	37029	73473	19.13%	2.162%
11	7.252	1919	1932	1945	rBV	157787	282574	73.58%	8.315%
12	7.326	1945	1955	1971	rVB	66797	124393	32.39%	3.660%
13	7.561	2019	2028	2040	rBV	22750	41964	10.93%	1.235%
14	7.882	2120	2128	2132	rBV3	4271	5471	1.42%	0.161%
15	8.037	2166	2176	2209	rBV	166382	350300	91.22%	10.308%
16	8.792	2398	2411	2431	rBV	186433	324122	84.40%	9.538%
17	9.506	2619	2633	2646	rBV7	5481	12602	3.28%	0.371%
18	10.162	2823	2837	2852	rBV	71242	115297	30.02%	3.393%
19	10.332	2880	2890	2902	rVB2	16851	27589	7.18%	0.812%
20	11.194	3146	3158	3179	rBV	194884	312136	81.28%	9.185%
21	11.509	3247	3256	3263	rBV10	2152	4317	1.12%	0.127%
22	11.570	3263	3275	3299	rVB	175160	284325	74.04%	8.367%
23	12.204	3464	3472	3483	rVB2	5326	8363	2.18%	0.246%
24	12.297	3491	3501	3511	rBV8	7369	12794	3.33%	0.376%
25	12.625	3597	3603	3611	rVB9	3029	4264	1.11%	0.125%




Sum of corrected areas: 3398332

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030494.D
Acq On : 11 Apr 2023 14:58
Operator : SY/MD
Sample : 02250-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

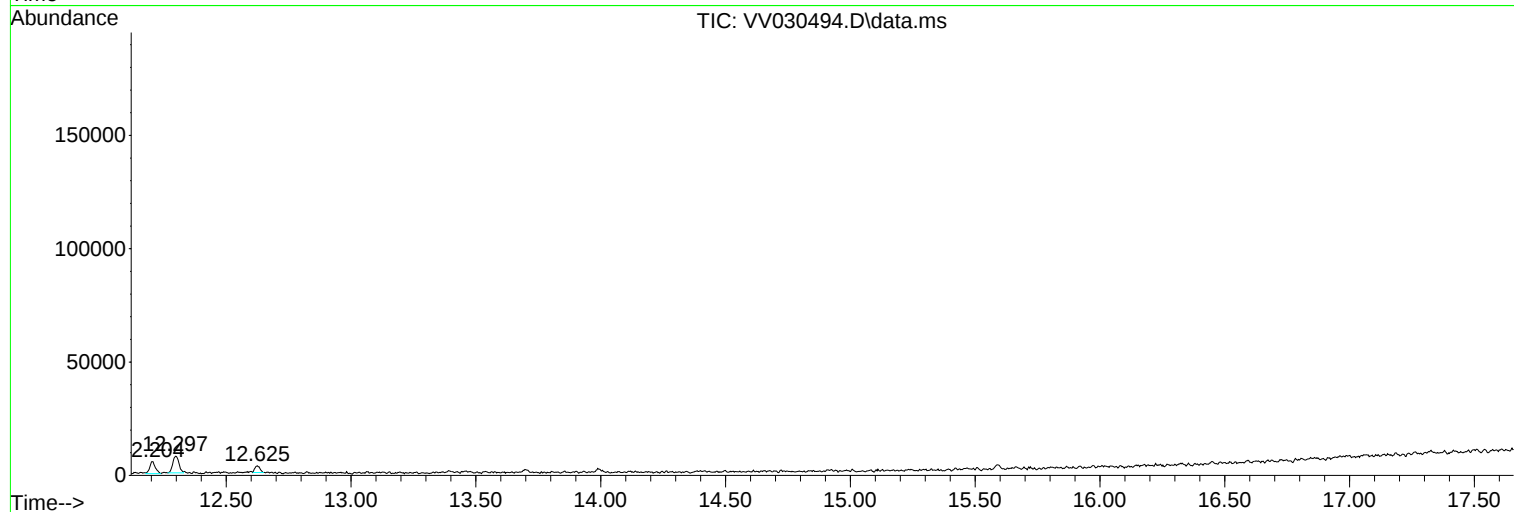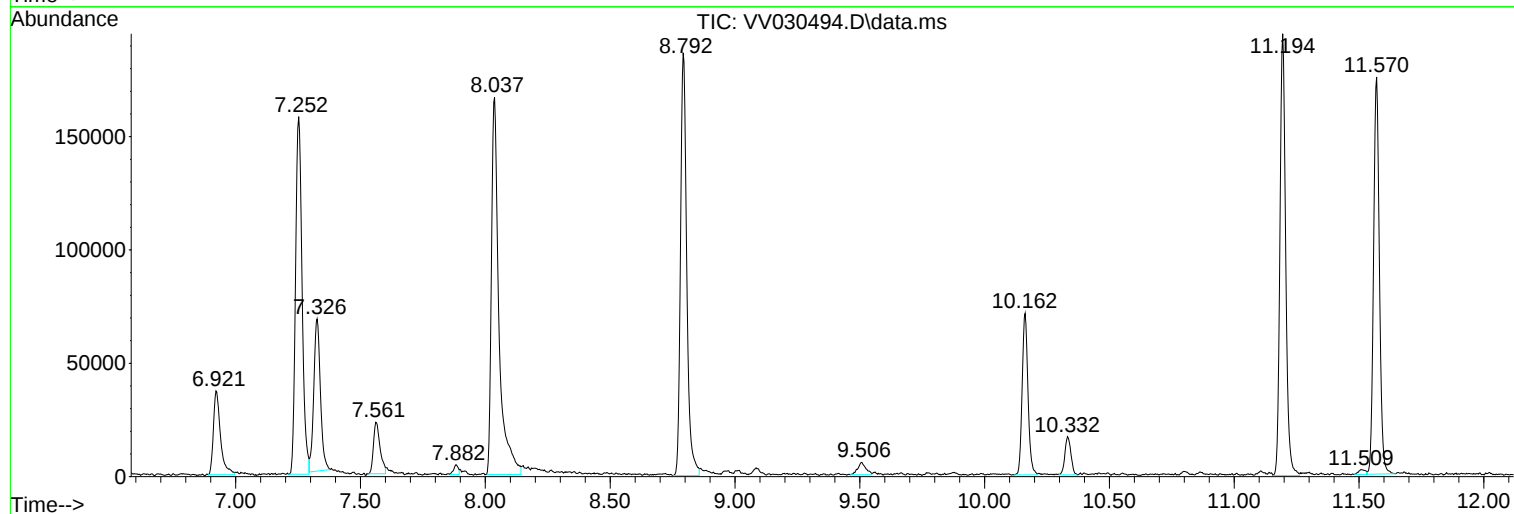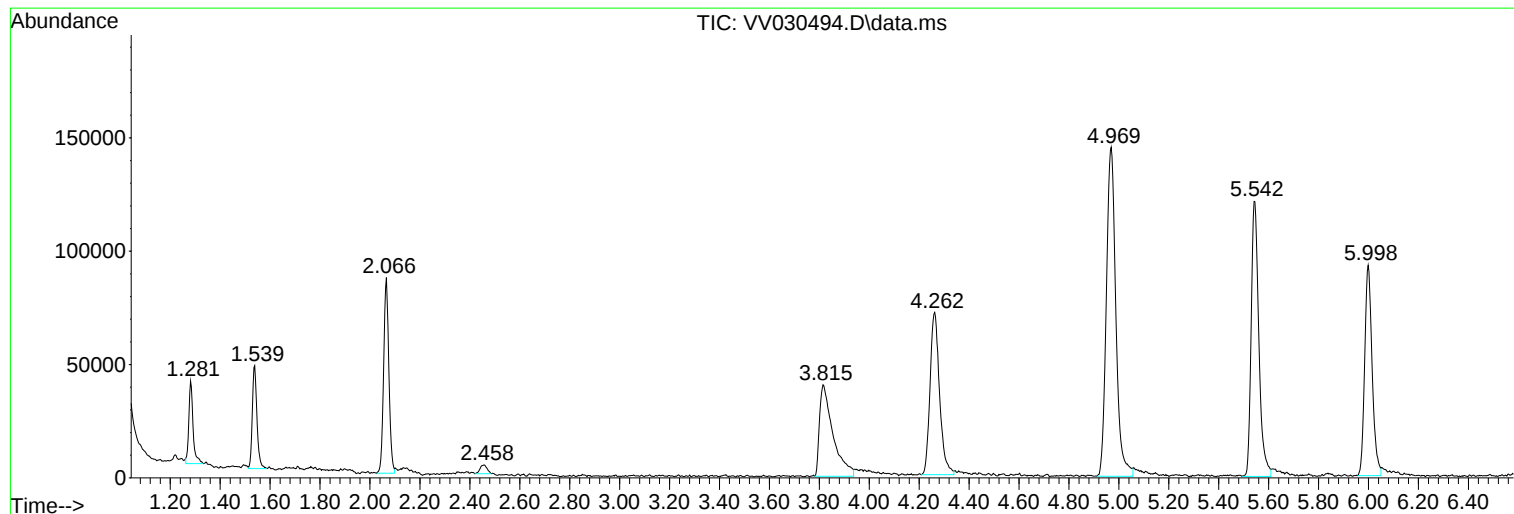

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030494.D
Acq On : 11 Apr 2023 14:58
Operator : SY/MD
Sample : 02250-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030494.D
Acq On : 11 Apr 2023 14:58
Operator : SY/MD
Sample : 02250-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc