

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030498.D
 Acq On : 11 Apr 2023 16:36
 Operator : SY/MD
 Sample : 02275-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rVB	22297	24740	8.93%	1.073%
2	1.539	147	155	163	rVB	26998	31399	11.33%	1.362%
3	2.063	308	318	333	rBV2	51347	75690	27.31%	3.283%
4	2.137	333	341	342	rBV7	2557	2797	1.01%	0.121%
5	2.455	429	440	460	rBV	51059	88902	32.08%	3.856%
6	3.822	853	865	887	rBV	31310	109929	39.67%	4.768%
7	4.259	985	1001	1026	rBV2	43795	118974	42.93%	5.160%
8	4.970	1202	1222	1245	rBV3	90280	241334	87.08%	10.467%
9	5.545	1388	1401	1422	rBV	74179	159673	57.62%	6.926%
10	5.998	1527	1542	1562	rBV3	57369	124739	45.01%	5.410%
11	6.924	1819	1830	1848	rBV2	24237	49710	17.94%	2.156%
12	7.252	1920	1932	1947	rBV	93767	169410	61.13%	7.348%
13	7.330	1947	1956	1967	rVB	18051	33444	12.07%	1.451%
14	7.564	2018	2029	2044	rBV2	15303	29289	10.57%	1.270%
15	7.883	2118	2128	2138	rBV2	9733	20166	7.28%	0.875%
16	8.037	2165	2176	2208	rBV	132714	277132	100.00%	12.020%
17	8.793	2399	2411	2431	rBV	117393	201294	72.63%	8.731%
18	9.510	2623	2634	2646	rBV	3249	7368	2.66%	0.320%
19	10.162	2826	2837	2849	rBV2	52707	87318	31.51%	3.787%
20	10.336	2879	2891	2901	rBV	28964	47687	17.21%	2.068%
21	11.111	3123	3132	3138	rBV8	2132	3761	1.36%	0.163%
22	11.194	3148	3158	3175	rBV	120841	193299	69.75%	8.384%
23	11.571	3263	3275	3291	rBV	105650	173373	62.56%	7.520%
24	11.661	3299	3303	3311	rVB	6516	5314	1.92%	0.230%
25	12.204	3462	3472	3481	rBV2	7000	11134	4.02%	0.483%
26	12.294	3492	3500	3512	rBV8	8675	14567	5.26%	0.632%
27	12.625	3598	3603	3610	rVB8	2282	3135	1.13%	0.136%




Sum of corrected areas: 2305578

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030498.D
Acq On : 11 Apr 2023 16:36
Operator : SY/MD
Sample : 02275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

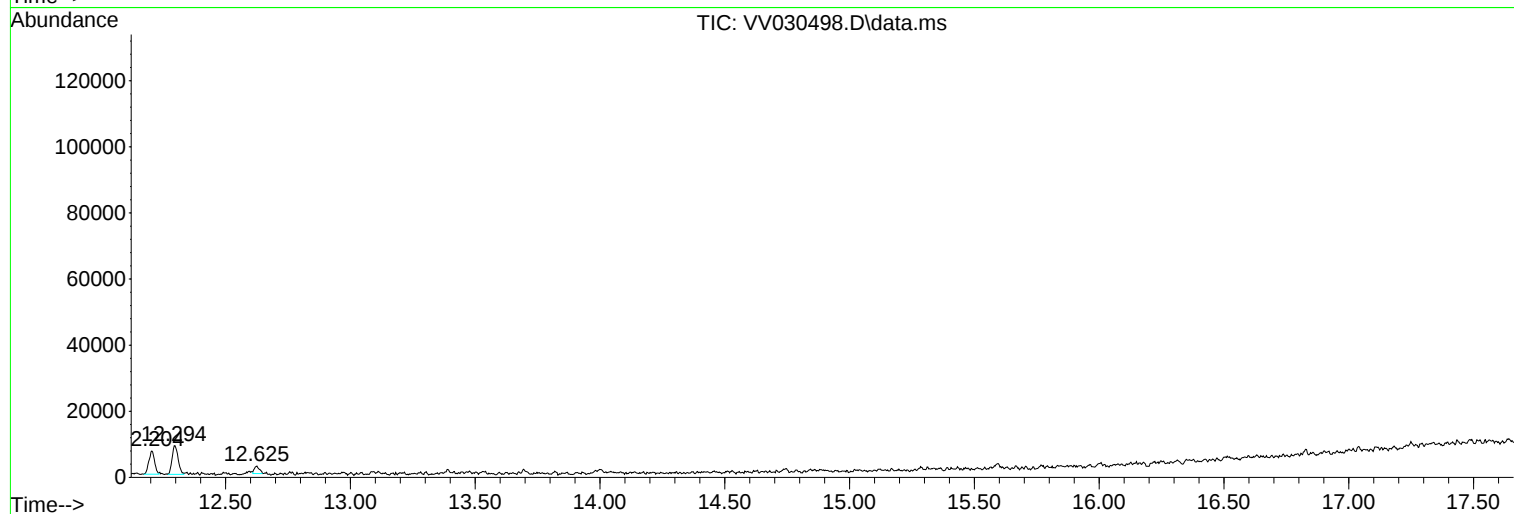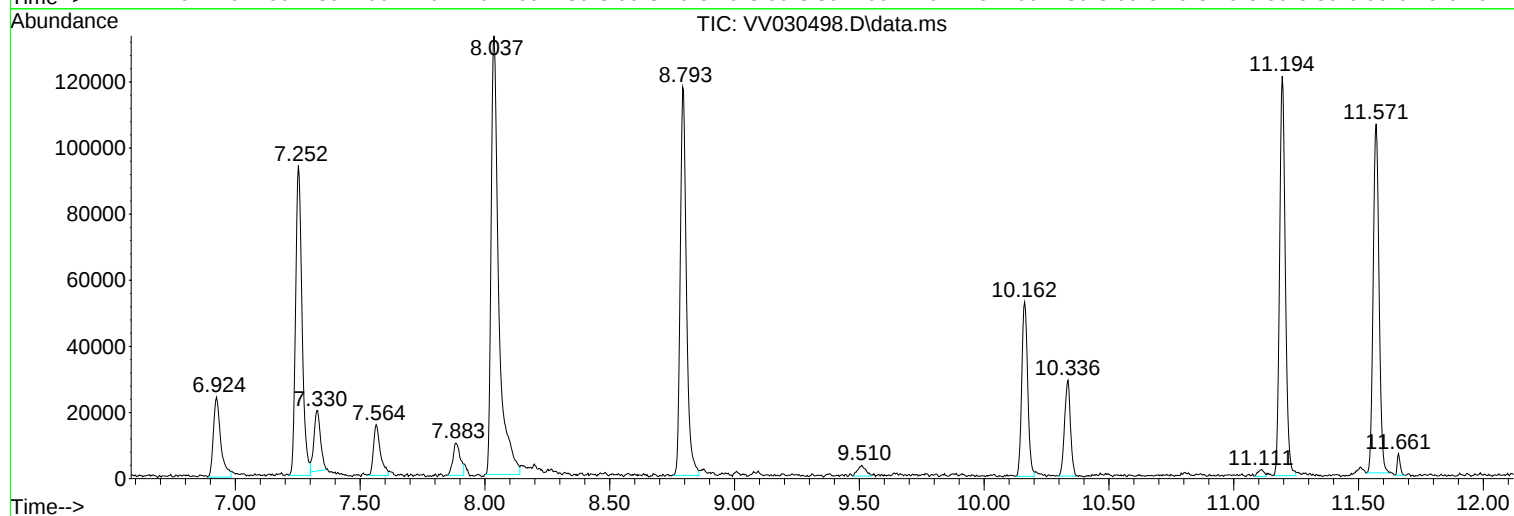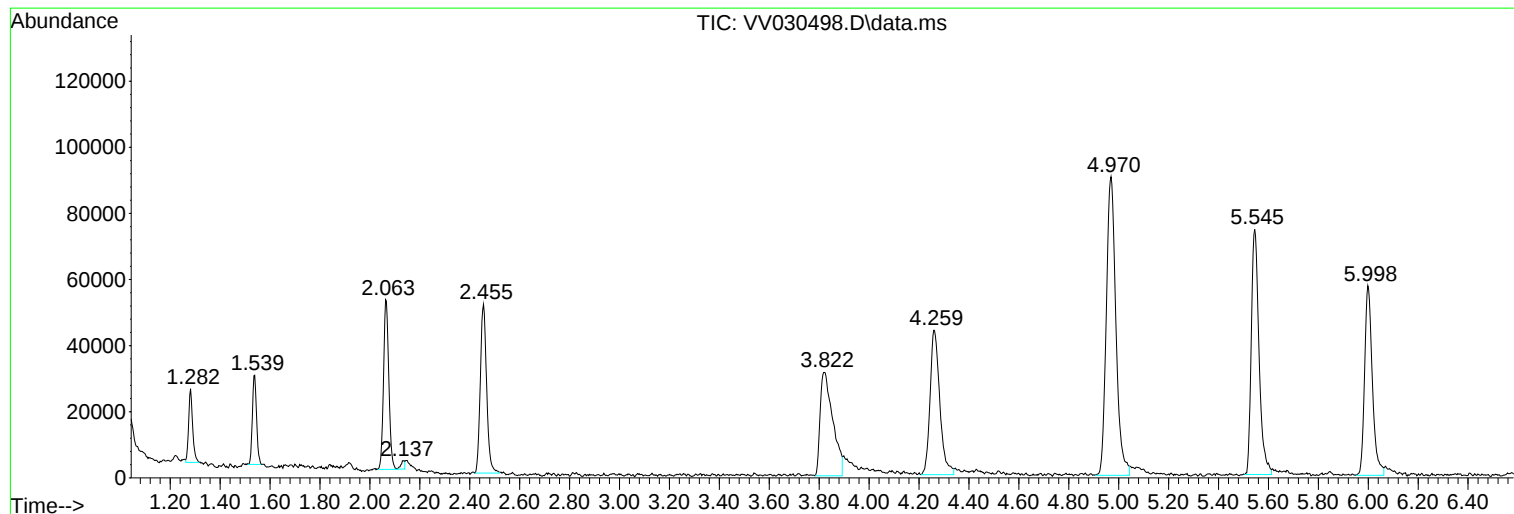

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030498.D
Acq On : 11 Apr 2023 16:36
Operator : SY/MD
Sample : 02275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030498.D
Acq On : 11 Apr 2023 16:36
Operator : SY/MD
Sample : 02275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------