

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030501.D
 Acq On : 11 Apr 2023 17:50
 Operator : SY/MD
 Sample : 02250-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	85	rBV	35296	36866	9.23%	1.049%
2	1.536	148	154	168	rVB	45038	55025	13.78%	1.565%
3	2.066	307	319	334	rBV	88262	131957	33.05%	3.753%
4	2.246	368	375	383	rVB2	3281	4222	1.06%	0.120%
5	2.455	430	440	450	rBV8	3141	5252	1.32%	0.149%
6	3.831	854	868	909	rBV2	33631	159762	40.01%	4.544%
7	4.259	985	1001	1025	rBV	73394	198186	49.63%	5.637%
8	4.969	1205	1222	1247	rBV3	151810	399303	100.00%	11.358%
9	5.542	1380	1400	1428	rBV	124107	267440	66.98%	7.607%
10	5.998	1529	1542	1562	rBV2	94648	206081	51.61%	5.862%
11	6.924	1819	1830	1853	rBV	38906	76215	19.09%	2.168%
12	7.252	1920	1932	1945	rBV	166244	291189	72.92%	8.283%
13	7.326	1947	1955	1971	rVB	45415	84311	21.11%	2.398%
14	7.561	2017	2028	2044	rBV2	23841	46607	11.67%	1.326%
15	7.886	2116	2129	2137	rBV3	7795	15013	3.76%	0.427%
16	8.037	2163	2176	2206	rBV	179612	388457	97.28%	11.049%
17	8.792	2399	2411	2436	rBV	194064	333078	83.41%	9.474%
18	9.513	2621	2635	2645	rBV	4130	9865	2.47%	0.281%
19	10.162	2827	2837	2854	rBV	77801	123279	30.87%	3.507%
20	10.333	2879	2890	2903	rVB2	21262	35904	8.99%	1.021%
21	11.194	3146	3158	3173	rBV	195153	310367	77.73%	8.828%
22	11.513	3248	3257	3263	rBV9	2197	4200	1.05%	0.119%
23	11.571	3263	3275	3294	rVV	182326	292066	73.14%	8.307%
24	12.204	3458	3472	3483	rBV2	6810	11826	2.96%	0.336%
25	12.297	3493	3501	3511	rBV5	11763	17492	4.38%	0.498%
26	12.625	3592	3603	3612	rVB5	3648	6291	1.58%	0.179%
27	13.998	4019	4030	4041	rVB3	2948	5440	1.36%	0.155%




Sum of corrected areas: 3515694

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030501.D
Acq On : 11 Apr 2023 17:50
Operator : SY/MD
Sample : 02250-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

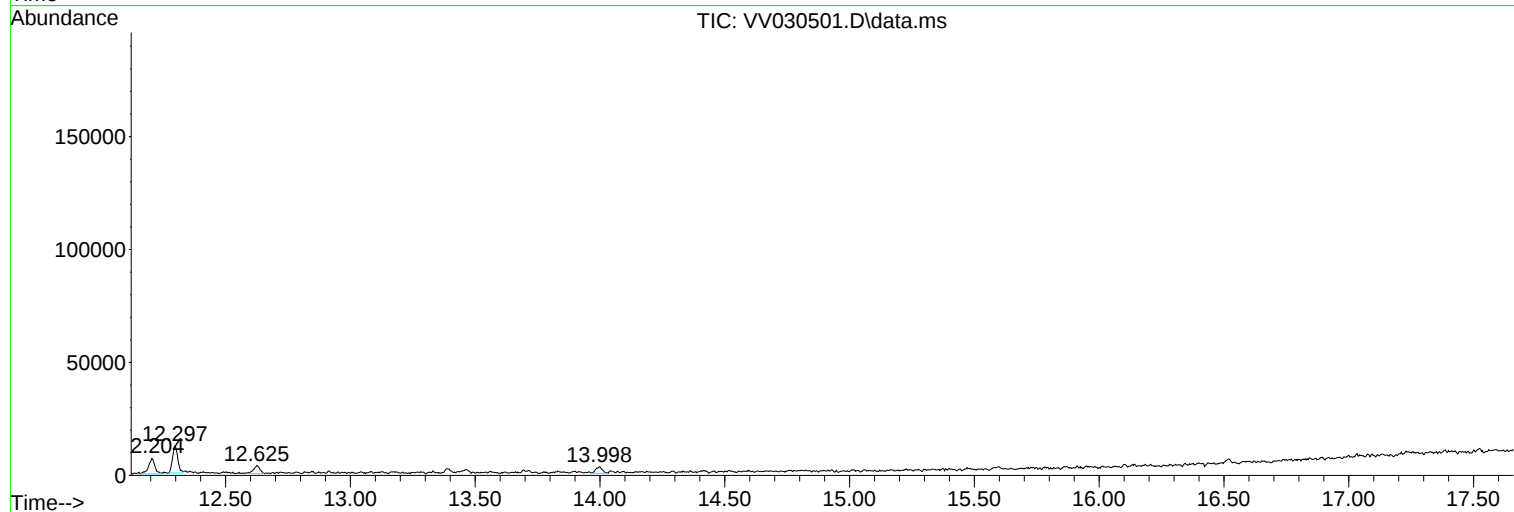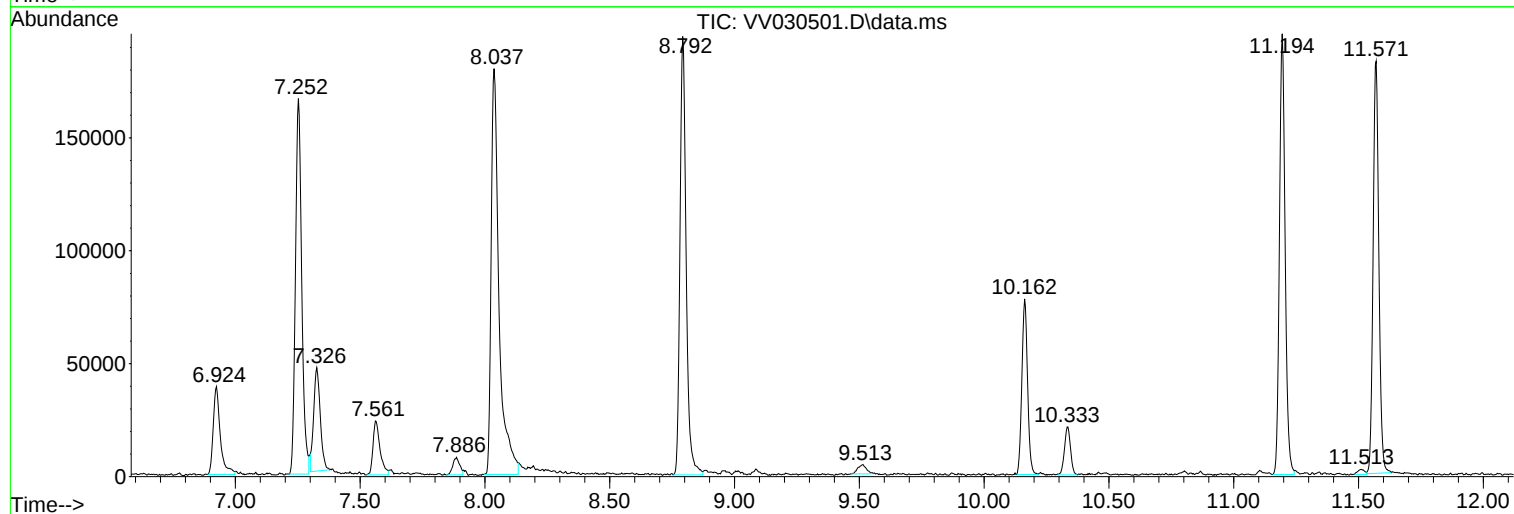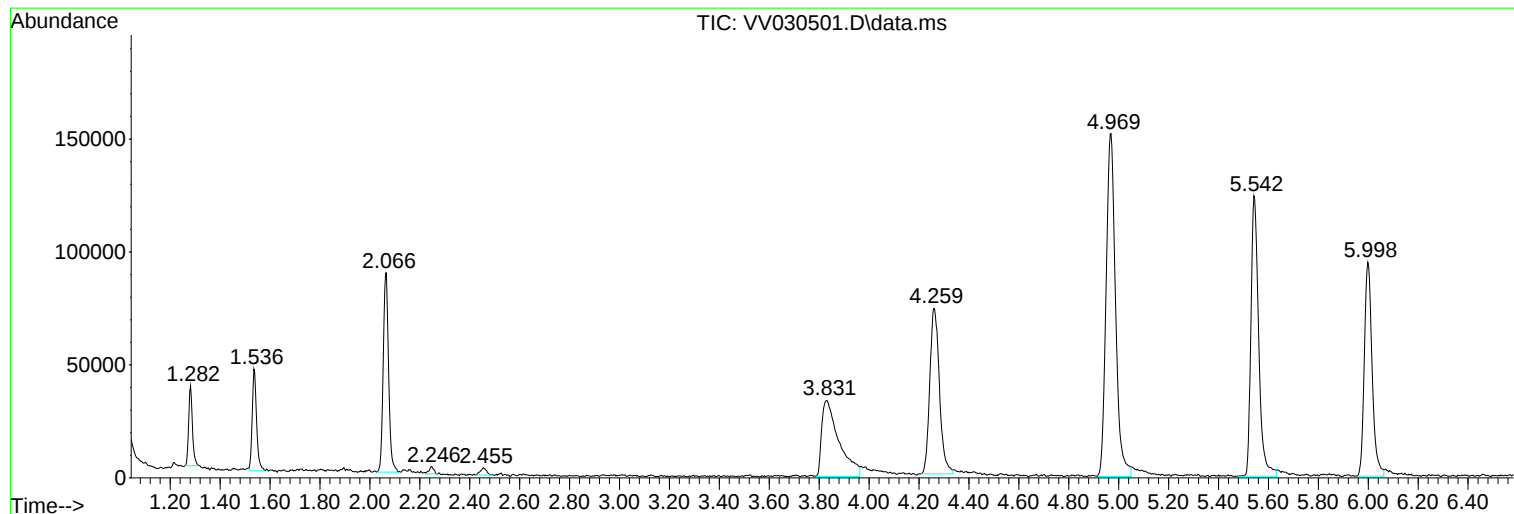

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030501.D
Acq On : 11 Apr 2023 17:50
Operator : SY/MD
Sample : 02250-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030501.D
Acq On : 11 Apr 2023 17:50
Operator : SY/MD
Sample : 02250-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------