

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
 Data File : VV030503.D
 Acq On : 11 Apr 2023 18:39
 Operator : SY/MD
 Sample : 02250-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	91	rVB	36777	42876	11.08%	1.294%
2	1.536	147	154	165	rVB	43804	50399	13.03%	1.520%
3	2.063	307	318	337	rBV	85606	124412	32.15%	3.753%
4	2.455	433	440	448	rBV4	3368	4875	1.26%	0.147%
5	3.825	854	866	893	rBV	37421	142295	36.77%	4.293%
6	4.259	981	1001	1024	rBV2	71400	192029	49.63%	5.793%
7	4.969	1204	1222	1248	rBV2	146780	386938	100.00%	11.674%
8	5.545	1386	1401	1420	rBV	122891	261568	67.60%	7.891%
9	5.998	1527	1542	1562	rBV2	94817	200515	51.82%	6.049%
10	6.921	1819	1829	1850	rBV	36733	75891	19.61%	2.290%
11	7.252	1918	1932	1949	rBV	159895	291600	75.36%	8.797%
12	7.564	2019	2029	2044	rBV2	23102	45141	11.67%	1.362%
13	7.883	2119	2128	2140	rBV2	9211	17135	4.43%	0.517%
14	8.037	2164	2176	2209	rBV	181206	382420	98.83%	11.537%
15	8.792	2399	2411	2431	rBV	188365	323155	83.52%	9.749%
16	10.162	2825	2837	2851	rBV	75371	121064	31.29%	3.652%
17	10.336	2880	2891	2903	rVB2	30997	50755	13.12%	1.531%
18	11.194	3146	3158	3176	rBV	190146	302489	78.18%	9.126%
19	11.570	3264	3275	3291	rBV	177625	283574	73.29%	8.555%
20	12.204	3462	3472	3483	rBV4	5848	10552	2.73%	0.318%
21	12.300	3494	3502	3508	rBV7	3662	4963	1.28%	0.150%




Sum of corrected areas: 3314646

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030503.D
Acq On : 11 Apr 2023 18:39
Operator : SY/MD
Sample : 02250-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

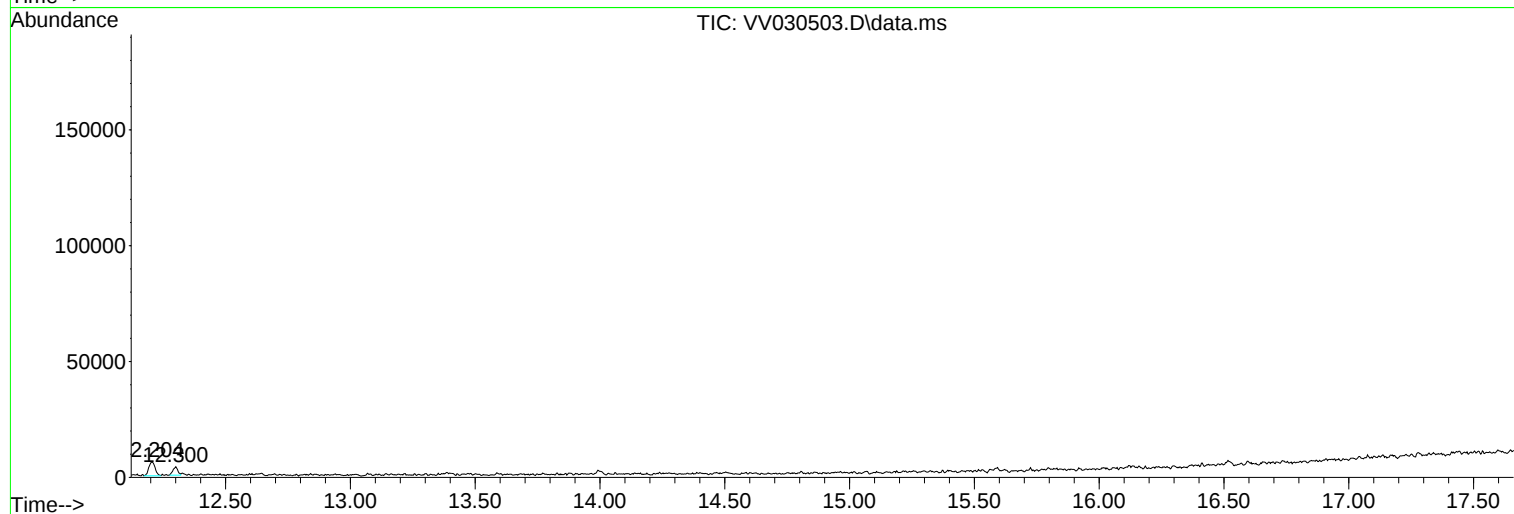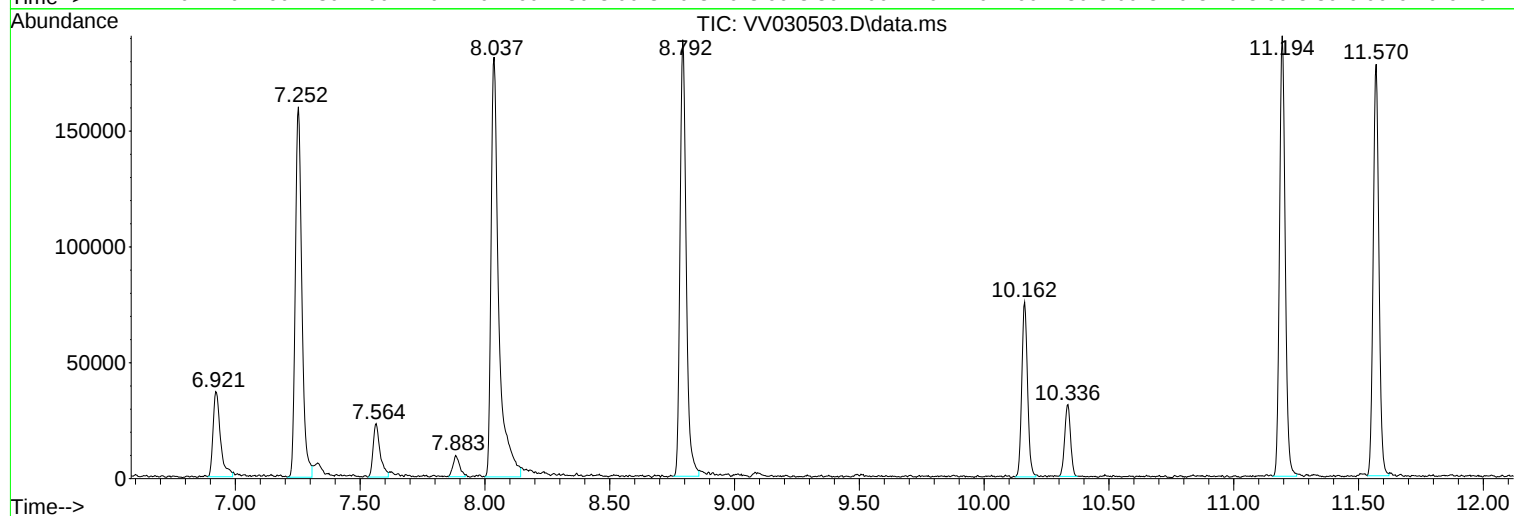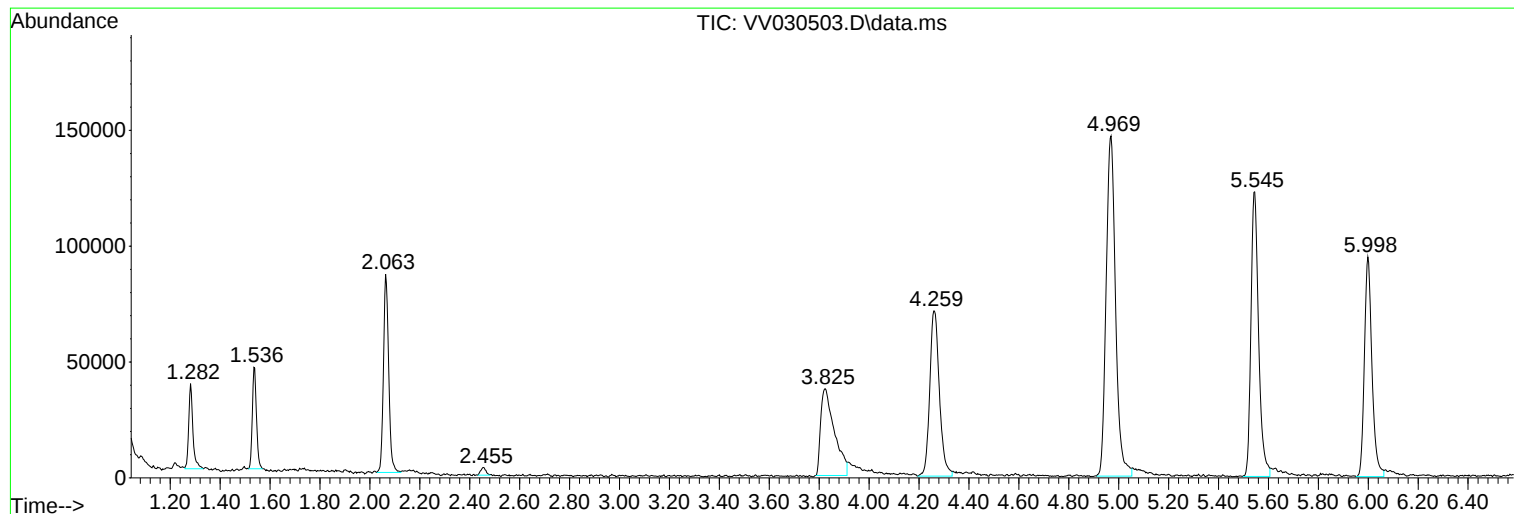

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030503.D
Acq On : 11 Apr 2023 18:39
Operator : SY/MD
Sample : 02250-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030503.D
Acq On : 11 Apr 2023 18:39
Operator : SY/MD
Sample : 02250-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc