


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041123\
Data File : VV030485.D
Acq On : 11 Apr 2023 09:21
Operator : SY/MD
Sample : BFB246
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB246

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 13 02:44:31 2023

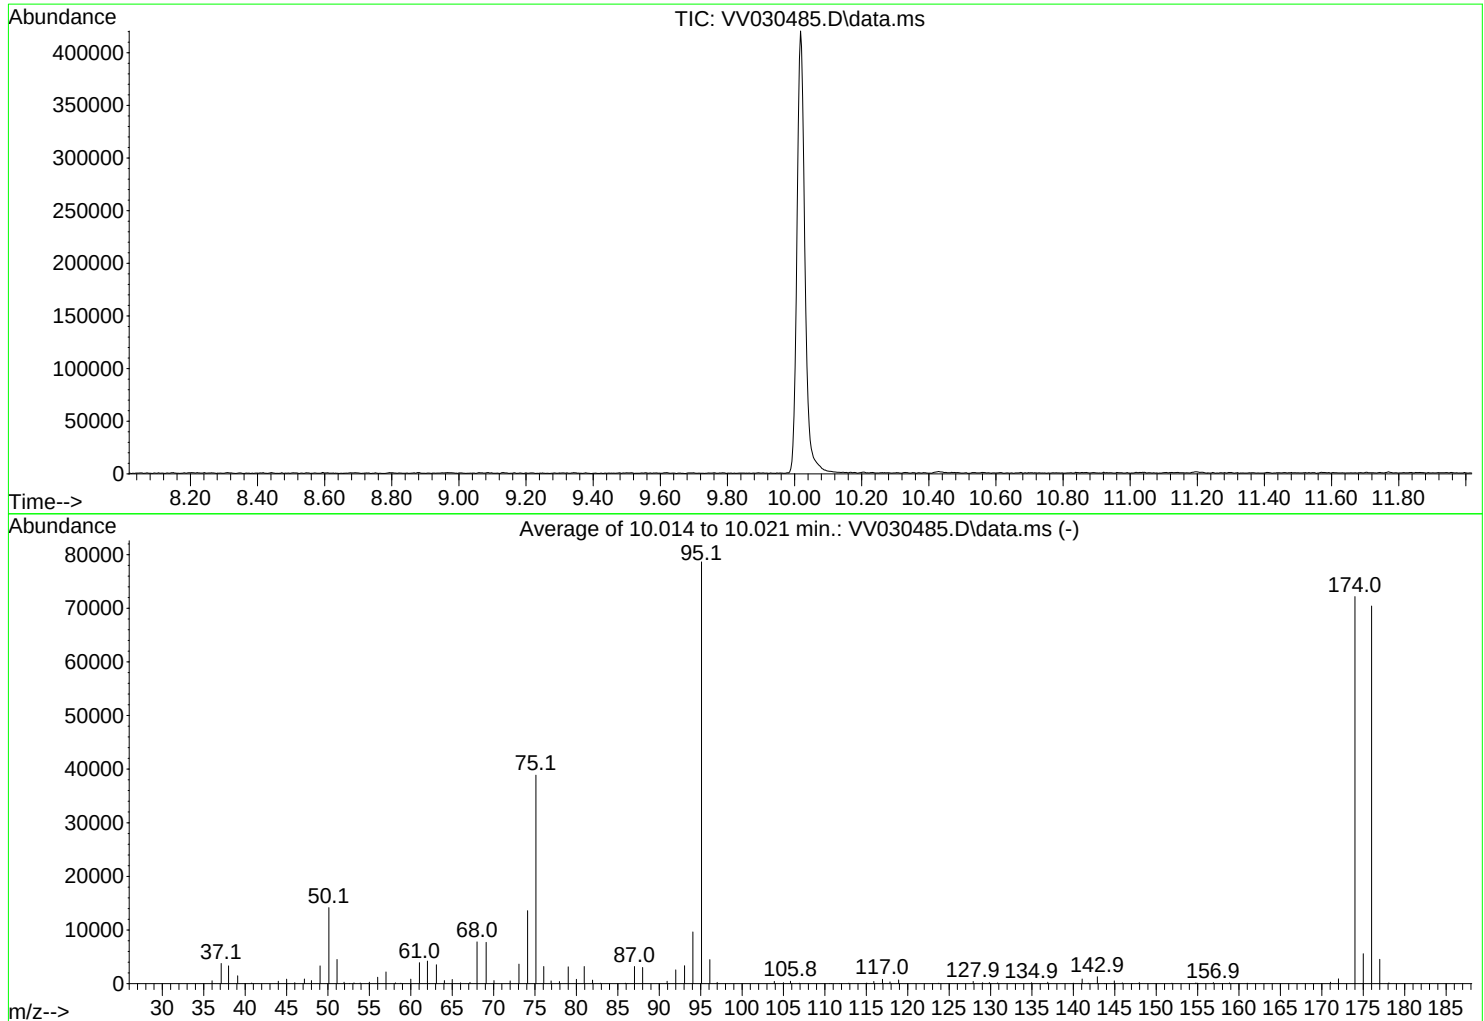

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	14165	PASS
75	95	30	80	49.4	38883	PASS
95	95	100	100	100.0	78651	PASS
96	95	5	9	5.7	4478	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.8	72179	PASS
175	174	5	9	7.7	5593	PASS
176	174	95	105	97.6	70424	PASS
177	176	5	10	6.4	4530	PASS

m/z	Abundance
35.90	127.0
40.00	198.0
44.10	210.0
44.60	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.00	747.0
37.10	3609.0
38.00	3136.0
39.10	1454.0
40.10	204.0
40.80	112.0
44.00	659.0
45.00	769.0
46.00	163.0
47.10	921.0
48.00	559.0
49.00	3371.0
50.10	13845.0
51.10	4353.0
52.00	261.0
53.10	138.0
53.80	121.0
55.00	286.0
56.00	1219.0
57.00	2153.0
58.10	102.0
58.80	123.0
60.00	766.0
61.00	3881.0
62.00	3936.0
63.10	3548.0
64.10	539.0
65.00	783.0
66.00	156.0
67.20	234.0
68.00	7722.0
69.10	7653.0
70.00	633.0
72.00	517.0
73.10	3563.0
74.10	13381.0
75.10	38368.0
76.00	3251.0
76.90	545.0
78.00	384.0
79.00	3039.0
80.00	801.0
81.00	3219.0
81.90	644.0
82.90	124.0
86.20	134.0
87.00	3309.0
88.00	2940.0
90.90	408.0
92.00	2392.0
93.10	3176.0
94.10	9116.0
95.10	76656.0
96.10	4433.0
97.00	257.0
103.90	368.0
105.00	160.0
105.90	421.0
106.90	115.0
111.80	110.0
115.00	131.0
115.90	389.0
116.90	847.0
117.90	344.0
118.90	720.0
123.80	136.0
127.90	390.0
129.00	169.0
130.00	216.0
130.80	139.0
134.90	175.0
136.90	257.0
140.00	121.0
141.00	832.0
142.90	1189.0
143.80	102.0
144.90	454.0
146.00	184.0
147.90	212.0
151.90	112.0
154.80	183.0
156.90	207.0
158.90	145.0
171.00	202.0
172.00	806.0
174.00	68136.0
175.00	5455.0
176.00	67176.0
177.00	4475.0
178.10	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.00	667.0
37.10	3887.0
38.00	3437.0
39.10	1510.0
40.10	229.0
40.80	123.0
44.00	690.0
45.00	880.0
46.00	191.0
47.20	864.0
48.00	595.0
49.10	3435.0
50.10	14650.0
51.10	4613.0
51.90	279.0
52.60	112.0
53.20	150.0
53.90	125.0
55.00	278.0
56.00	1217.0
57.00	2242.0
58.20	139.0
58.80	112.0
60.00	848.0
61.00	4014.0
62.00	4369.0
63.10	3655.0
64.00	581.0
65.00	805.0
66.00	180.0
67.10	246.0
68.00	8150.0
69.10	7959.0
70.00	572.0
72.00	504.0
73.00	3737.0
74.10	14035.0
75.10	40264.0
76.00	3231.0
76.90	500.0
77.90	407.0
79.00	3239.0
80.00	829.0
81.00	3313.0
82.00	664.0
82.90	115.0
85.90	132.0
87.00	3313.0
88.00	3129.0
90.90	452.0
92.00	2661.0
93.00	3443.0
94.00	9915.0
95.10	81400.0
96.10	4594.0
97.00	239.0
103.90	441.0
105.00	179.0
105.80	481.0
106.90	101.0
110.60	102.0
112.90	115.0
115.10	132.0
115.90	439.0
116.90	830.0
117.90	343.0
118.90	703.0
123.70	124.0
127.90	438.0
129.10	174.0
129.80	204.0
130.90	159.0
135.00	175.0
136.90	271.0
140.00	106.0
141.10	908.0
141.80	109.0
142.90	1314.0
145.00	538.0
145.90	138.0
147.10	105.0
148.00	218.0
151.90	116.0
154.80	228.0
156.90	235.0
158.90	141.0
161.00	146.0
171.00	270.0
172.00	950.0
174.00	74360.0
175.00	5743.0
176.00	72912.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

177.004618.0

178.10159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.10	580.0
37.10	3767.0
38.00	3356.0
39.10	1443.0
40.00	224.0
40.80	103.0
44.00	625.0
45.00	825.0
46.00	206.0
47.10	811.0
48.00	566.0
49.10	3106.0
50.10	14001.0
51.10	4568.0
51.90	257.0
53.20	147.0
54.00	139.0
55.00	245.0
56.00	1183.0
57.00	2158.0
58.20	175.0
60.00	869.0
61.10	3796.0
62.00	4284.0
63.10	3366.0
64.00	578.0
65.00	745.0
66.00	158.0
67.10	238.0
68.00	7525.0
69.10	7491.0
70.10	506.0
72.00	485.0
73.00	3601.0
74.10	13407.0
75.10	38016.0
76.10	3081.0
77.00	450.0
77.90	385.0
79.00	3131.0
80.00	779.0
80.90	3067.0
82.00	656.0
85.90	138.0
87.00	2920.0
88.00	2952.0
91.00	500.0
92.00	2633.0
93.00	3411.0
94.00	9866.0
95.10	77896.0
96.10	4408.0
97.00	191.0
103.90	473.0
105.00	181.0
105.80	428.0
106.90	101.0
110.80	101.0
112.90	137.0
115.10	139.0
115.90	390.0
117.00	764.0
117.80	336.0
118.90	605.0
127.90	403.0
129.10	172.0
129.80	245.0
130.90	167.0
135.00	173.0
136.90	251.0
141.00	855.0
141.80	129.0
142.90	1333.0
144.90	554.0
145.80	124.0
148.00	204.0
155.00	254.0
156.90	219.0
158.80	136.0
161.00	162.0
171.10	329.0
172.00	942.0
174.00	74040.0
175.00	5582.0
176.00	71184.0
177.00	4498.0
178.10	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246