




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035131.D
Acq On : 11 Apr 2024 18:09
Operator : SY/MD
Sample : P2056-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

Quant Time: Apr 12 01:22:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

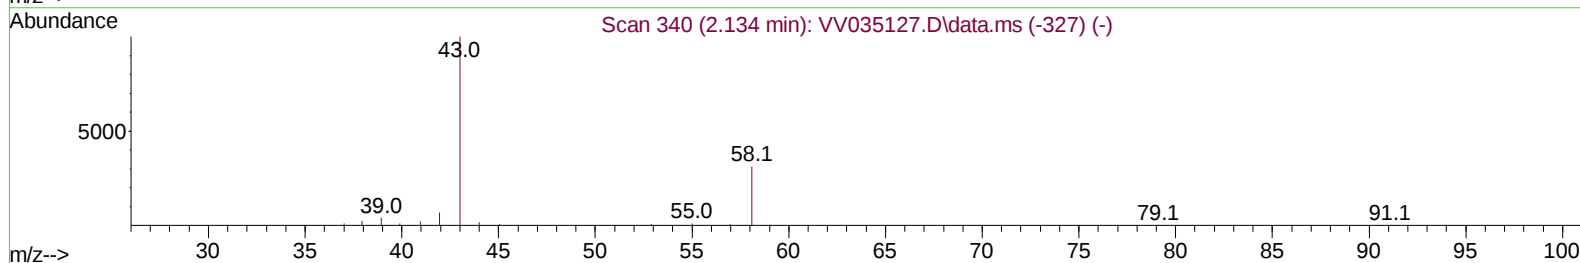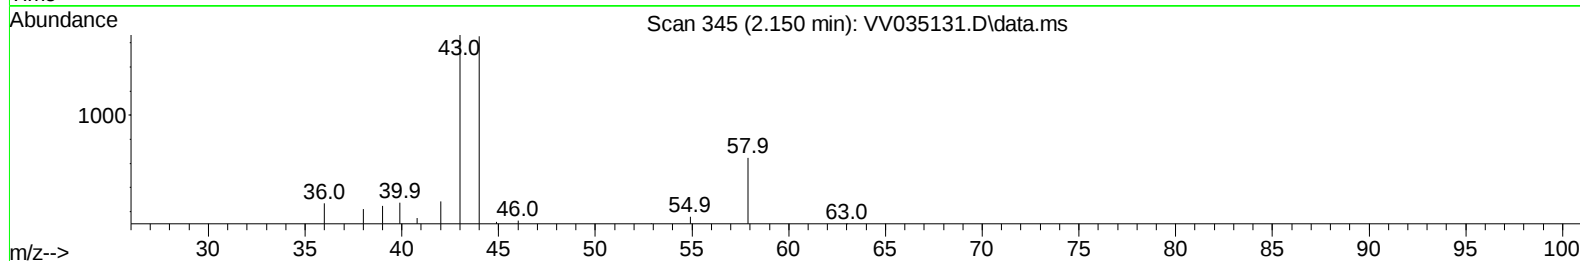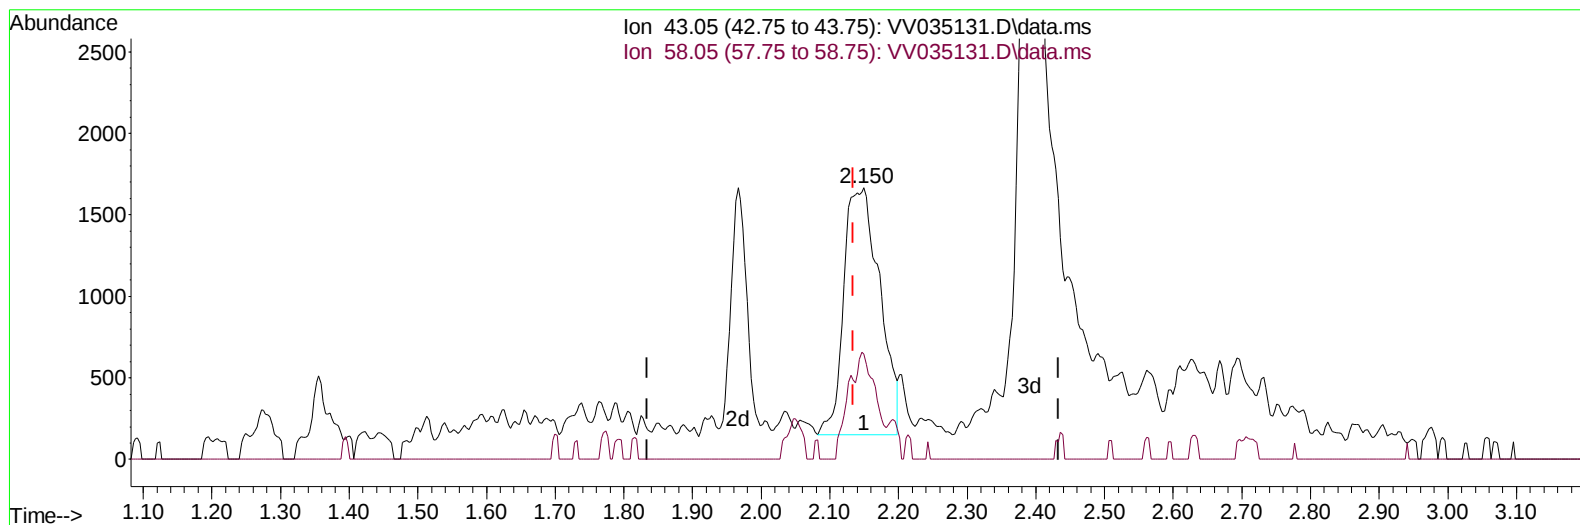

TIC: VV035131.D\data.ms

(13) Acetone (T)

2.150min (+ 0.016) 5.03 ug/L

response 5502

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	22.06
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035131.D
Acq On : 11 Apr 2024 18:09
Operator : SY/MD
Sample : P2056-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP4

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:22:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

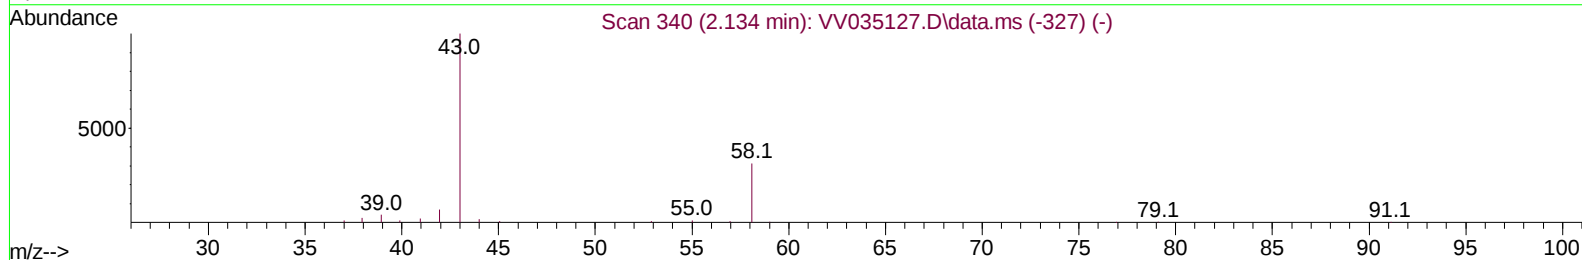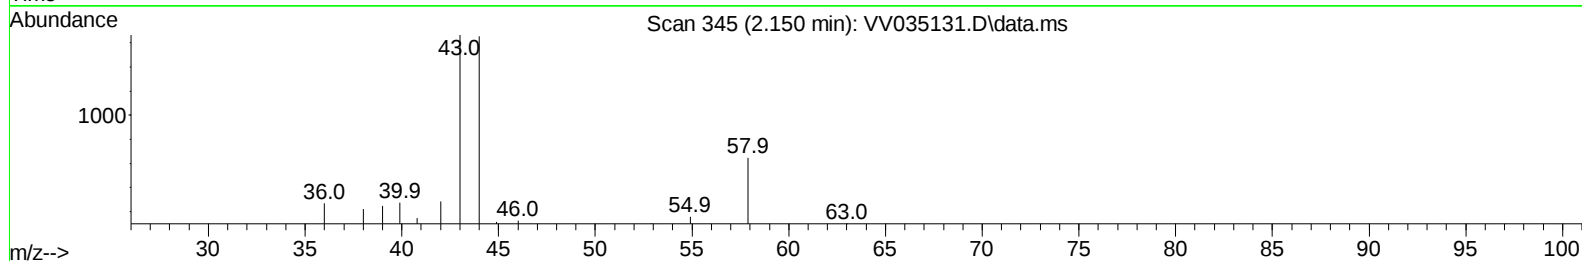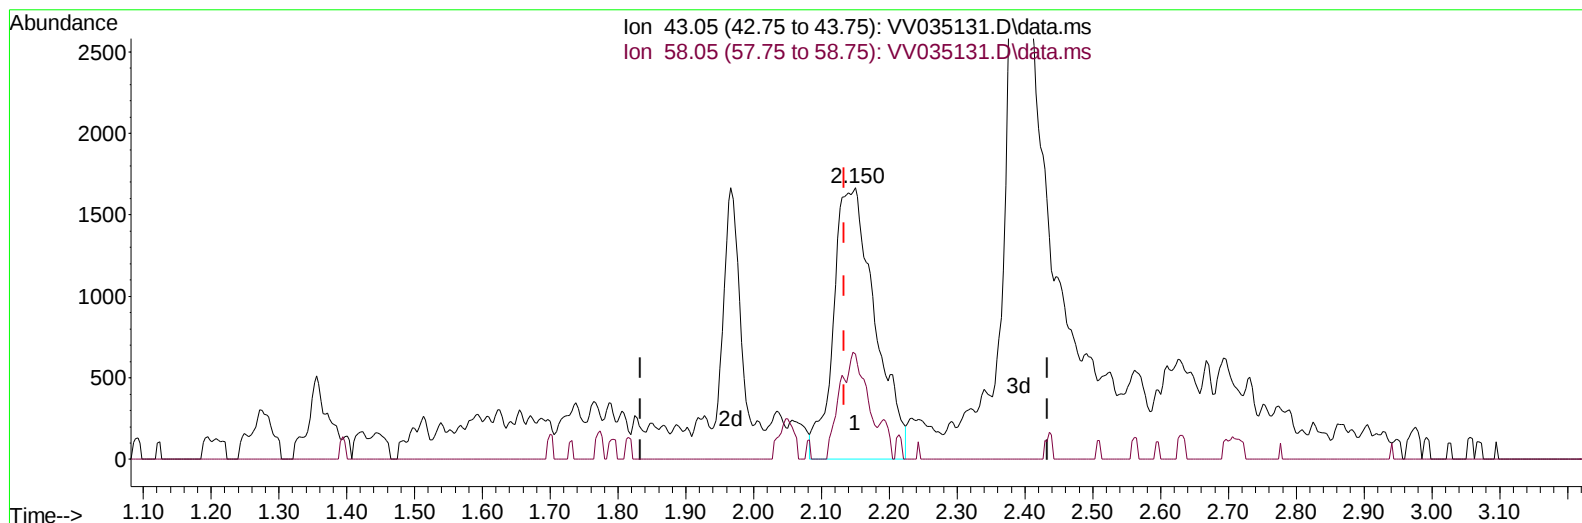

TIC: VV035131.D\data.ms

(13) Acetone (T)

2.150min (+ 0.016) 6.48 ug/L m

response 7080

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	17.15
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035131.D
 Acq On : 11 Apr 2024 18:09
 Operator : SY/MD
 Sample : P2056-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBP4

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:22:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
 Supervised By :Semsettin Yesilyurt 04/16/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.539	114		116230	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		118987	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		51418	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		40697	4.249	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	85.000%	
7) Chloroethane-d5	1.532	69		39272	4.973	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	99.400%	
11) 1,1-Dichloroethene-d2	2.057	65		19822	4.556	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	91.200%	
20) 2-Butanone-d5	3.812	46		142766	95.256	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	190.520%#	
24) Chloroform-d	4.249	84		80348	5.184	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	103.600%	
26) 1,2-Dichloroethane-d4	4.947	65		46528	6.647	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	133.000%#	
32) Benzene-d6	4.960	84		157373	5.056	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	101.200%	
36) 1,2-Dichloropropane-d6	5.989	67		52880	5.789	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	115.800%	
41) Toluene-d8	7.246	98		126195	4.463	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	89.200%	
43) trans-1,3-Dichloroprop...	7.564	79		17494	5.391	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	107.800%	
46) 2-Hexanone-d5	8.027	63		105049	94.317	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	188.640%#	
56) 1,1,2,2-Tetrachloroeth...	10.153	84		47636	7.473	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	149.400%#	
66) 1,2-Dichlorobenzene-d4	11.561	152		48945	6.043	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	120.800%#	
Target Compounds							
						Qvalue	
13) Acetone	2.150	43		7080m	6.476	ug/L	
15) Methyl Acetate	2.391	43		12788	4.238	ug/L #	89
16) Methylene chloride	2.446	84		3871	0.400	ug/L	89
47) Tetrachloroethene	7.905	164	2854555	400.307	ug/L		97
65) 1,4-Dichlorobenzene	11.210	146		4586	0.279	ug/L	97
67) 1,2-Dichlorobenzene	11.577	146		2485	0.164	ug/L	93
70) 1,2,4-trichlorobenzene	13.204	180		2336	0.244	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035131.D
Acq On : 11 Apr 2024 18:09
Operator : SY/MD
Sample : P2056-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP4

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:22:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

