




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035134.D
 Acq On : 11 Apr 2024 19:20
 Operator : SY/MD
 Sample : P2056-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP7

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:22:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
 Supervised By :Semsettin Yesilyurt 04/16/2024

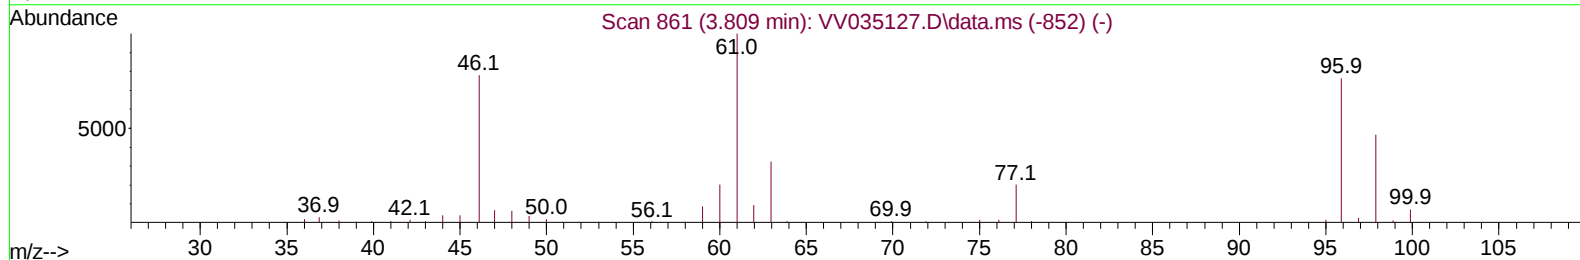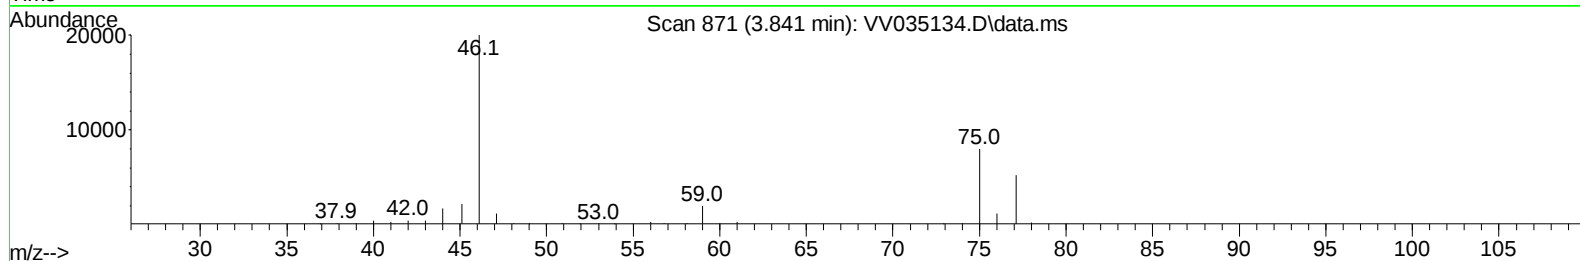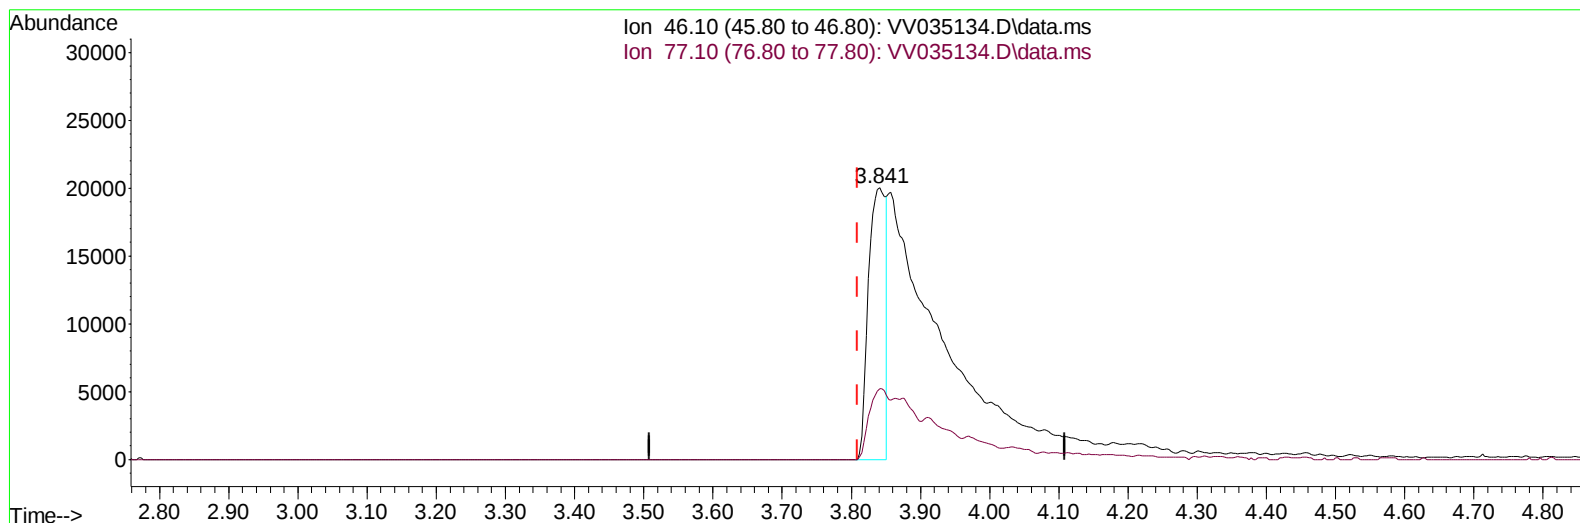

TIC: VV035134.D\data.ms

(20) 2-Butanone-d5 (S)

3.841min (+ 0.032) 15.24 ug/L

response 34988

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	17.20	30.02#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035134.D
Acq On : 11 Apr 2024 19:20
Operator : SY/MD
Sample : P2056-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP7

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:22:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

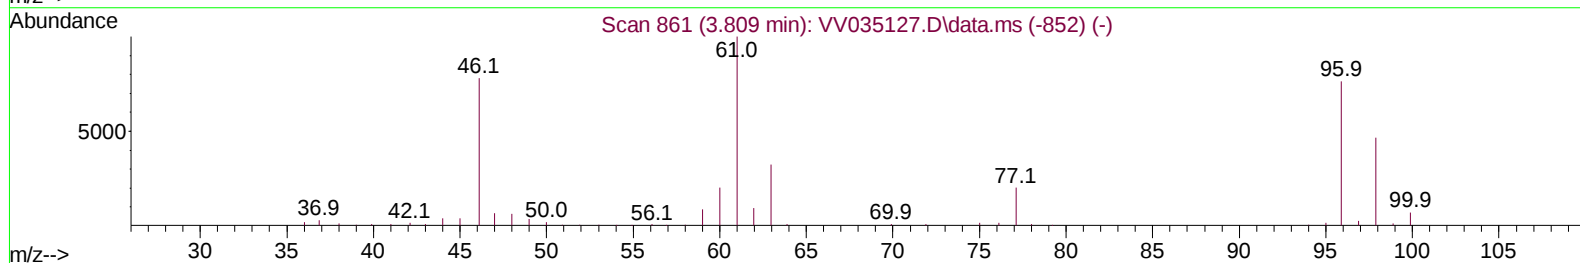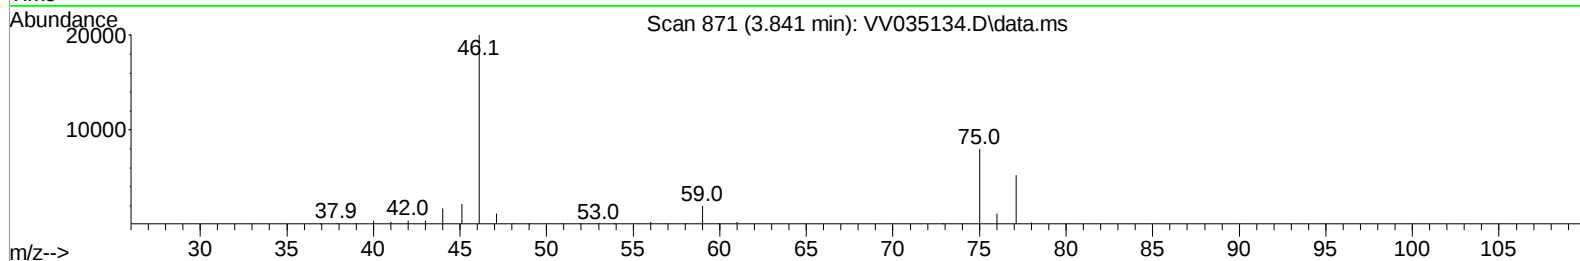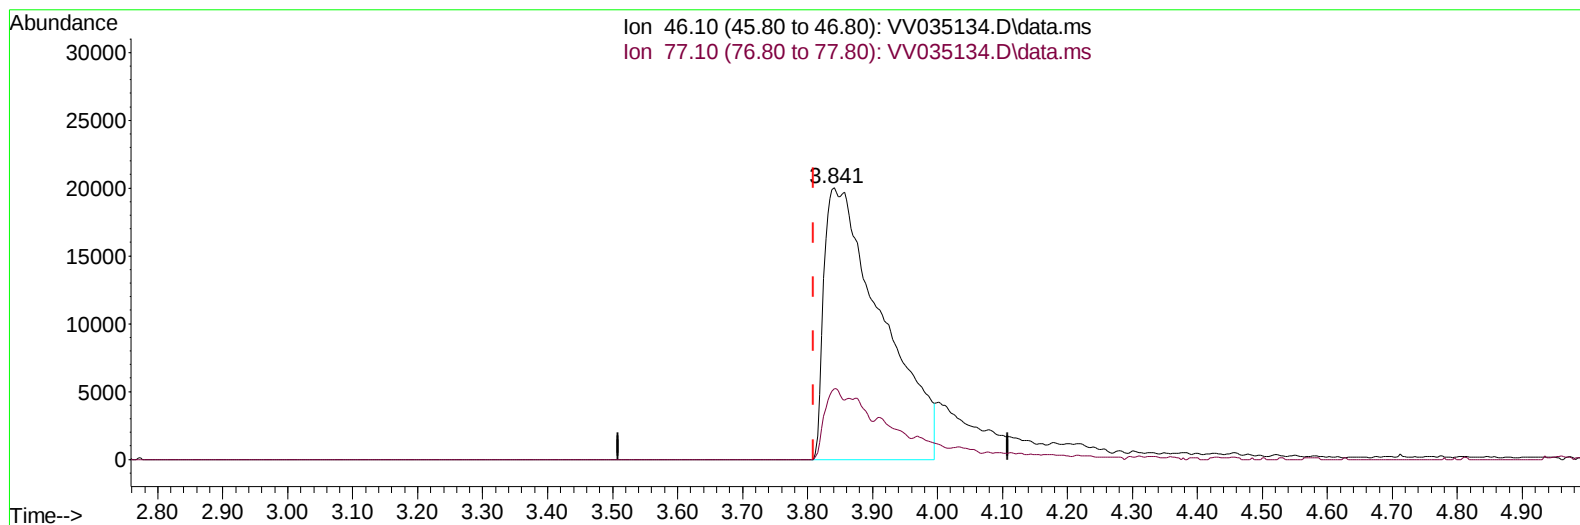

TIC: VV035134.D\data.ms

(20) 2-Butanone-d5 (S)

3.841min (+ 0.032) 53.87 ug/L m

response 123662

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	17.20	8.49#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035134.D
 Acq On : 11 Apr 2024 19:20
 Operator : SY/MD
 Sample : P2056-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP7

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:22:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
 Supervised By :Semsettin Yesilyurt 04/16/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	178015	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	180164	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	78016	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	60505	4.124	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.400%
7) Chloroethane-d5	1.532	69	58528	4.839	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.800%
11) 1,1-Dichloroethene-d2	2.056	65	28350	4.255	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.000%
20) 2-Butanone-d5	3.841	46	123662m	53.872	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.740%
24) Chloroform-d	4.246	84	119453	5.032	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	4.944	65	60036	5.600	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.000%
32) Benzene-d6	4.960	84	231231	4.906	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
36) 1,2-Dichloropropane-d6	5.989	67	77396	5.595	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.000%
41) Toluene-d8	7.243	98	188795	4.410	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%
43) trans-1,3-Dichloroprop...	7.561	79	22396	4.558	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%
46) 2-Hexanone-d5	8.031	63	89040	52.798	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.600%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	54860	5.684	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.600%
66) 1,2-Dichlorobenzene-d4	11.561	152	66748	5.432	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.600%
Target Compounds						Qvalue
47) Tetrachloroethene	7.905	164	48047	4.450	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035134.D
Acq On : 11 Apr 2024 19:20
Operator : SY/MD
Sample : P2056-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP7

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:22:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

