




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035140.D
Acq On : 11 Apr 2024 21:42
Operator : SY/MD
Sample : P2056-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BW3

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:24:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

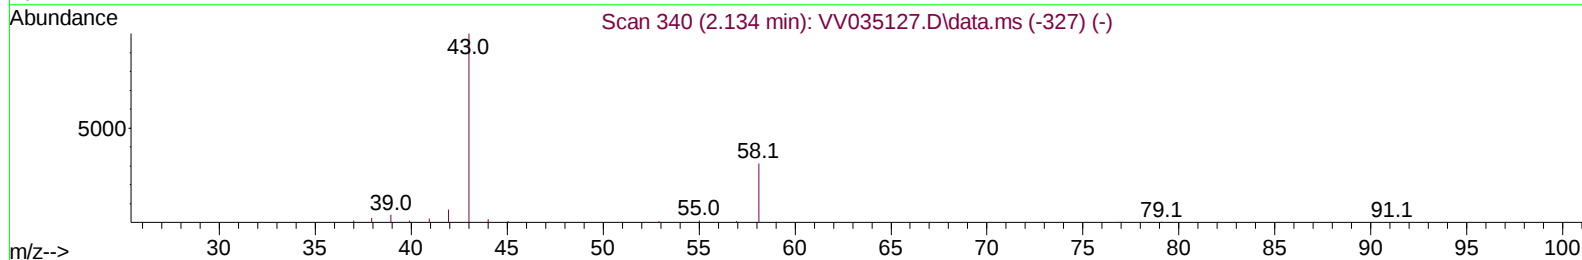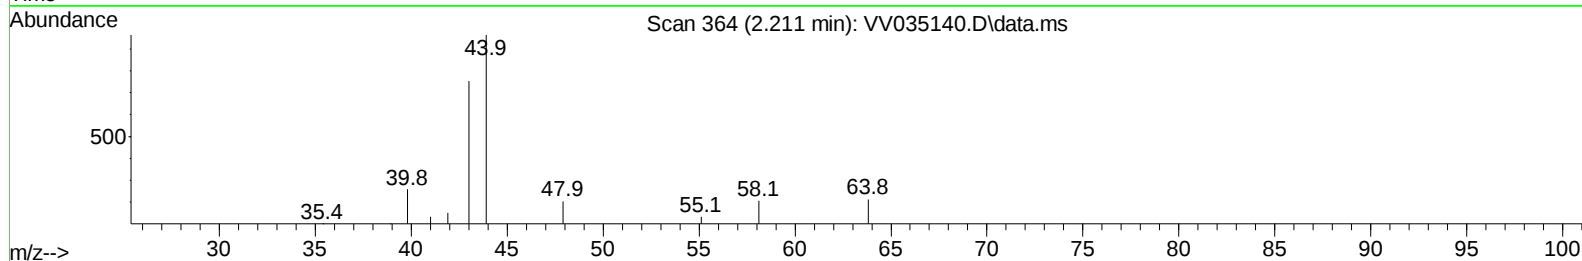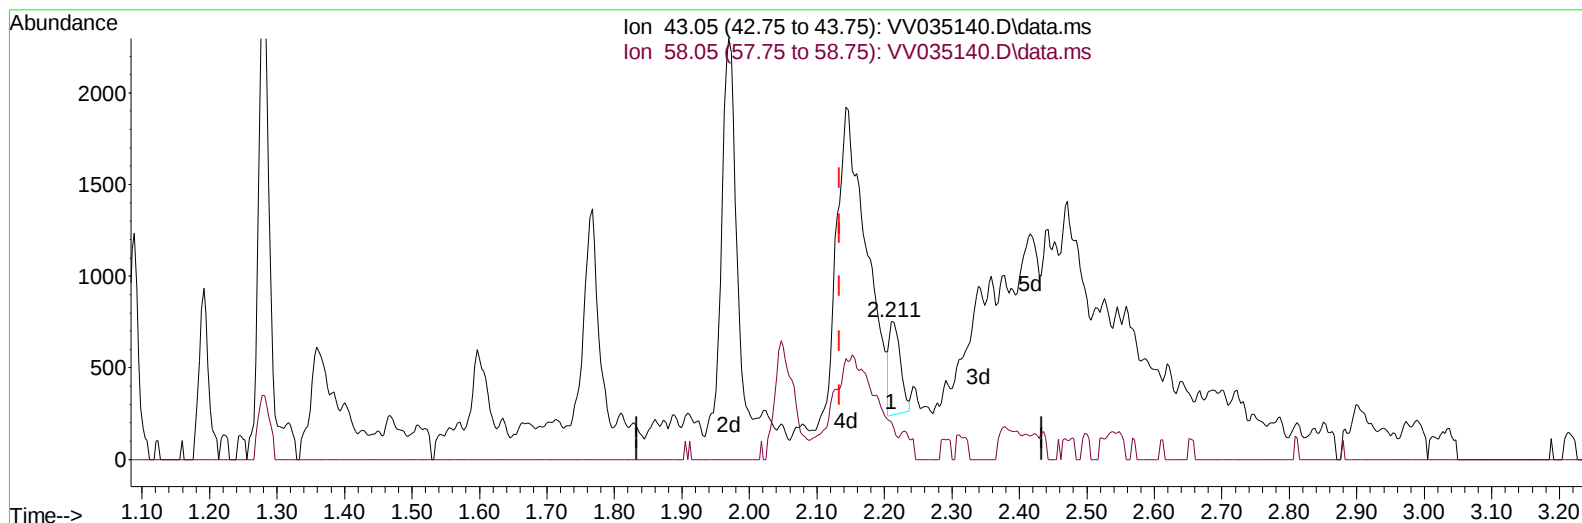

TIC: VV035140.D\data.ms

(13) Acetone (T)

2.211min (+ 0.077) 0.47 ug/L

response 585

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	30.09
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035140.D
Acq On : 11 Apr 2024 21:42
Operator : SY/MD
Sample : P2056-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BW3

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:24:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

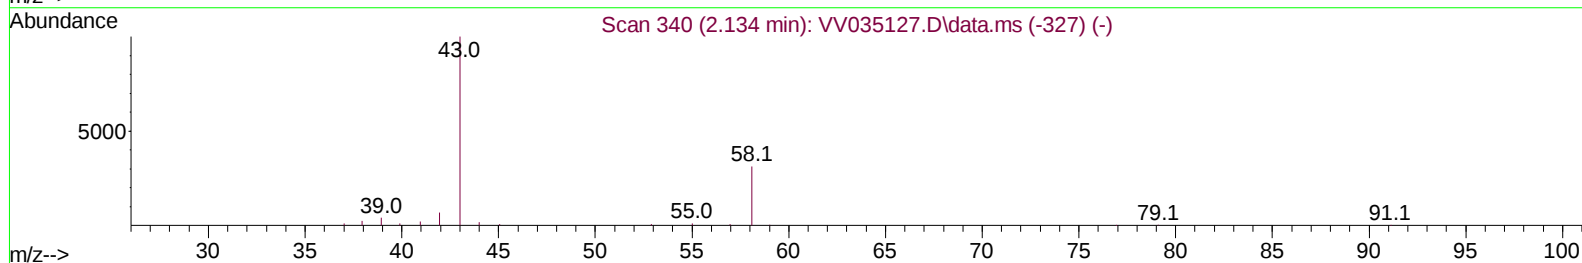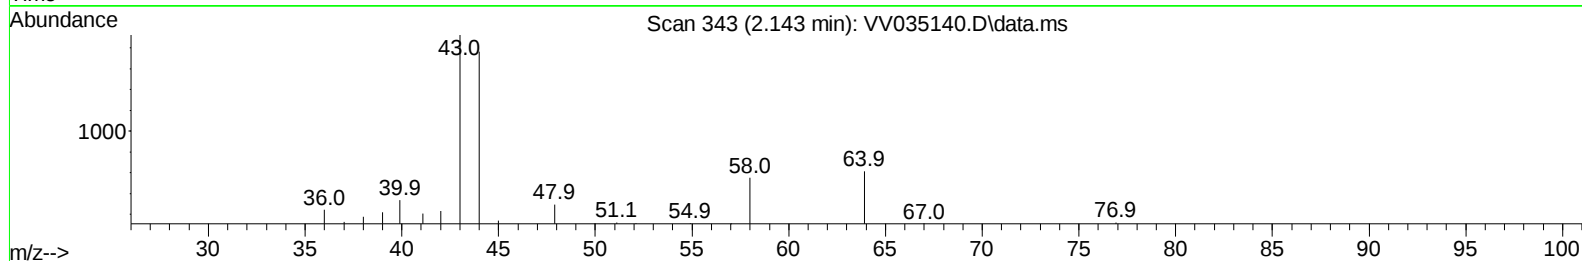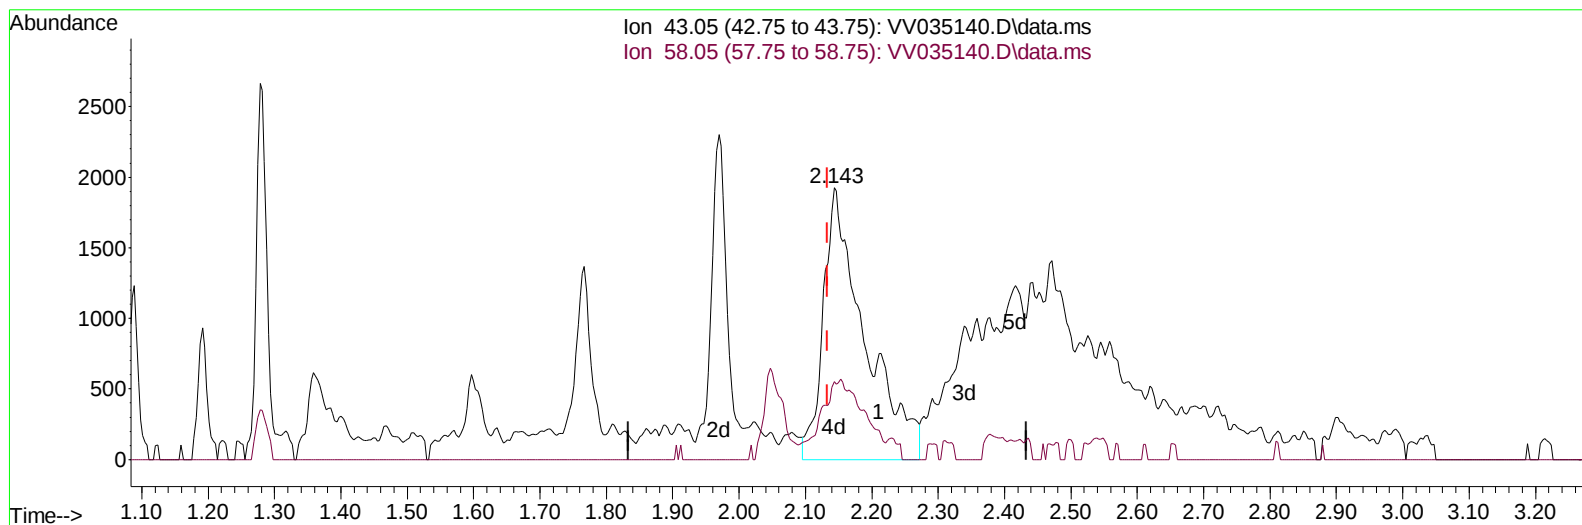

TIC: VV035140.D\data.ms

(13) Acetone (T)

2.143min (+ 0.009) 6.65 ug/L m

response 8324

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	2.11
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035140.D
 Acq On : 11 Apr 2024 21:42
 Operator : SY/MD
 Sample : P2056-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BW3

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:24:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
 Supervised By :Semsettin Yesilyurt 04/16/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.538	114		133013	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		136931	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		58382	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		45884	4.186	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.800%	
7) Chloroethane-d5	1.532	69		45172	4.998	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.000%	
11) 1,1-Dichloroethene-d2	2.059	65		23176	4.655	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.000%	
20) 2-Butanone-d5	3.818	46		134736	78.555	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	157.120%#	
24) Chloroform-d	4.252	84		92653	5.224	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.400%	
26) 1,2-Dichloroethane-d4	4.947	65		52769	6.588	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	131.800%#	
32) Benzene-d6	4.960	84		178504	4.983	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%	
36) 1,2-Dichloropropane-d6	5.992	67		59538	5.663	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.200%	
41) Toluene-d8	7.246	98		140433	4.316	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.400%	
43) trans-1,3-Dichloroprop...	7.564	79		16094	4.309	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.200%	
46) 2-Hexanone-d5	8.027	63		94242	73.526	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	147.060%#	
56) 1,1,2,2-Tetrachloroeth...	10.152	84		52495	7.157	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	143.200%#	
66) 1,2-Dichlorobenzene-d4	11.561	152		52701	5.731	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.600%	
Target Compounds							
13) Acetone	2.143	43		8324m	6.653	ug/L	
47) Tetrachloroethene	7.918	164		2127	0.259	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035140.D
Acq On : 11 Apr 2024 21:42
Operator : SY/MD
Sample : P2056-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BW3

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:24:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

