




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035153.D
Acq On : 12 Apr 2024 03:42
Operator : SY/MD
Sample : P2057-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBM8

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:55:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:02:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

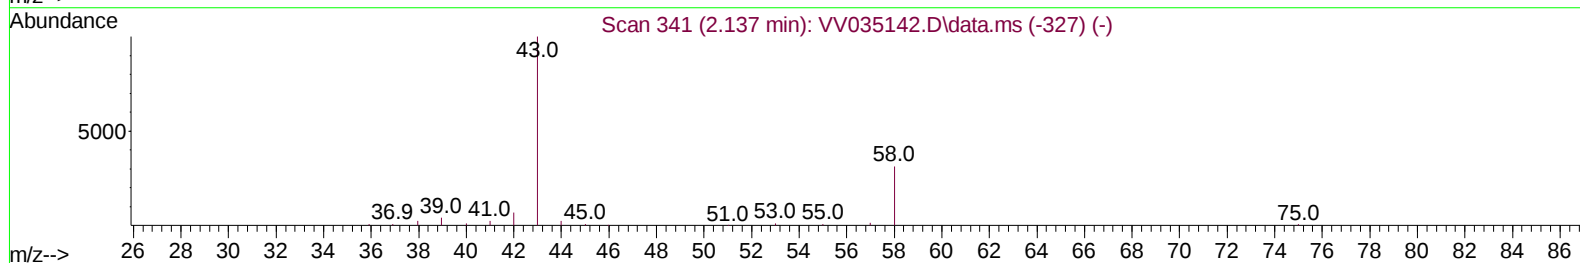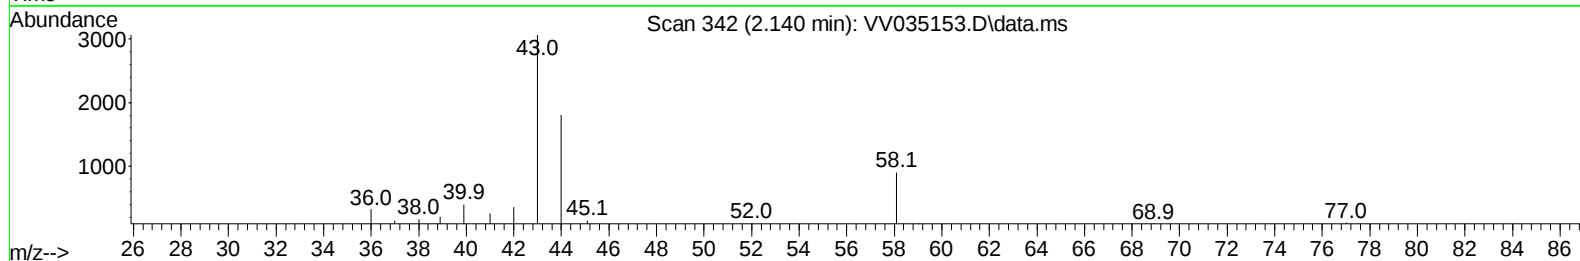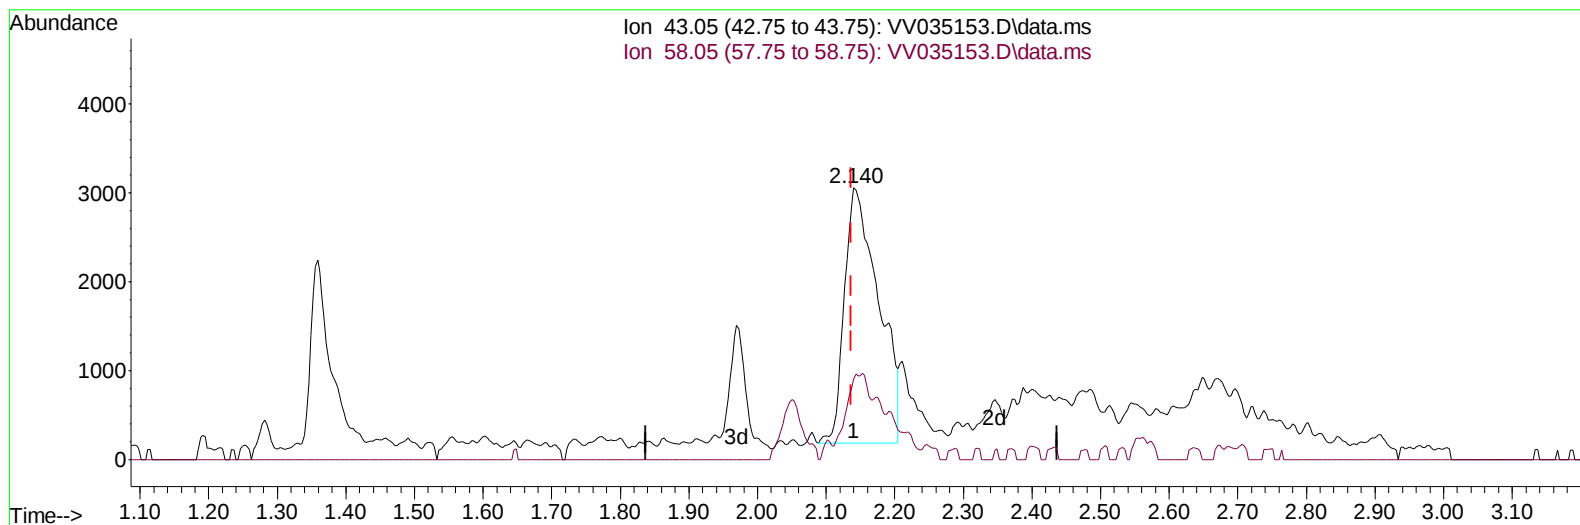

TIC: VV035153.D\data.ms

(13) Acetone (T)

2.140min (+ 0.003) 6.15 ug/L

response 9928

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	17.59
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035153.D
Acq On : 12 Apr 2024 03:42
Operator : SY/MD
Sample : P2057-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBM8

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:55:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:02:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

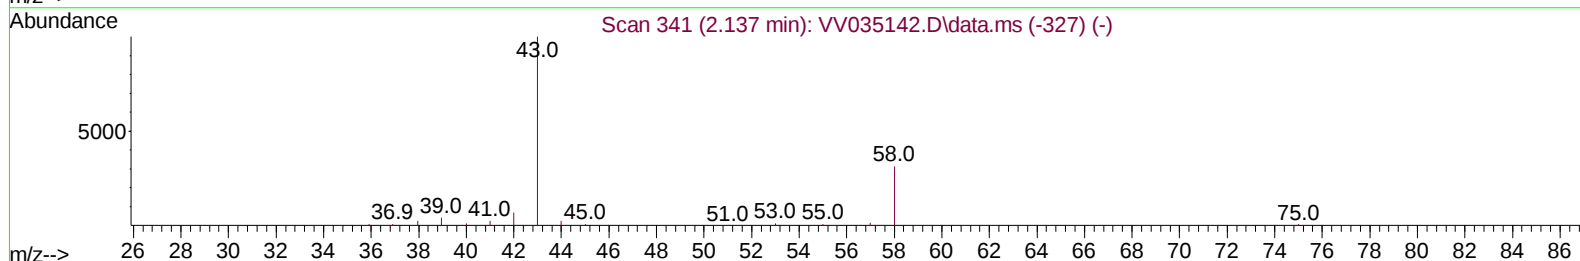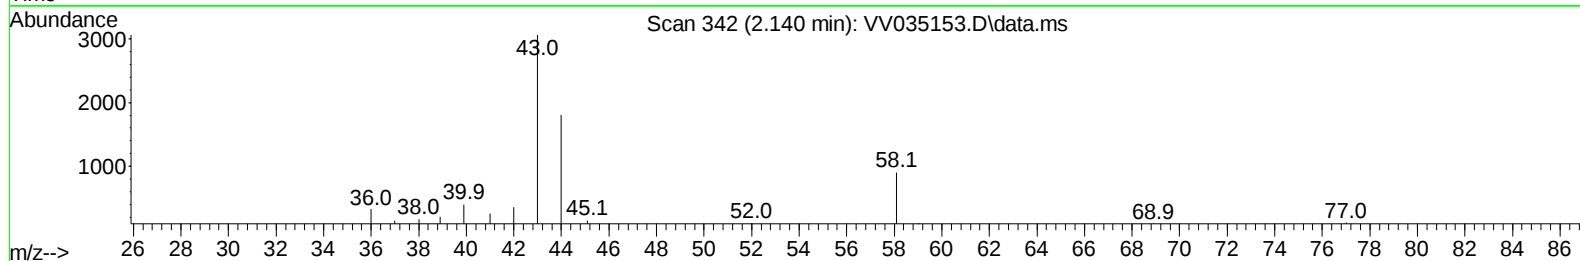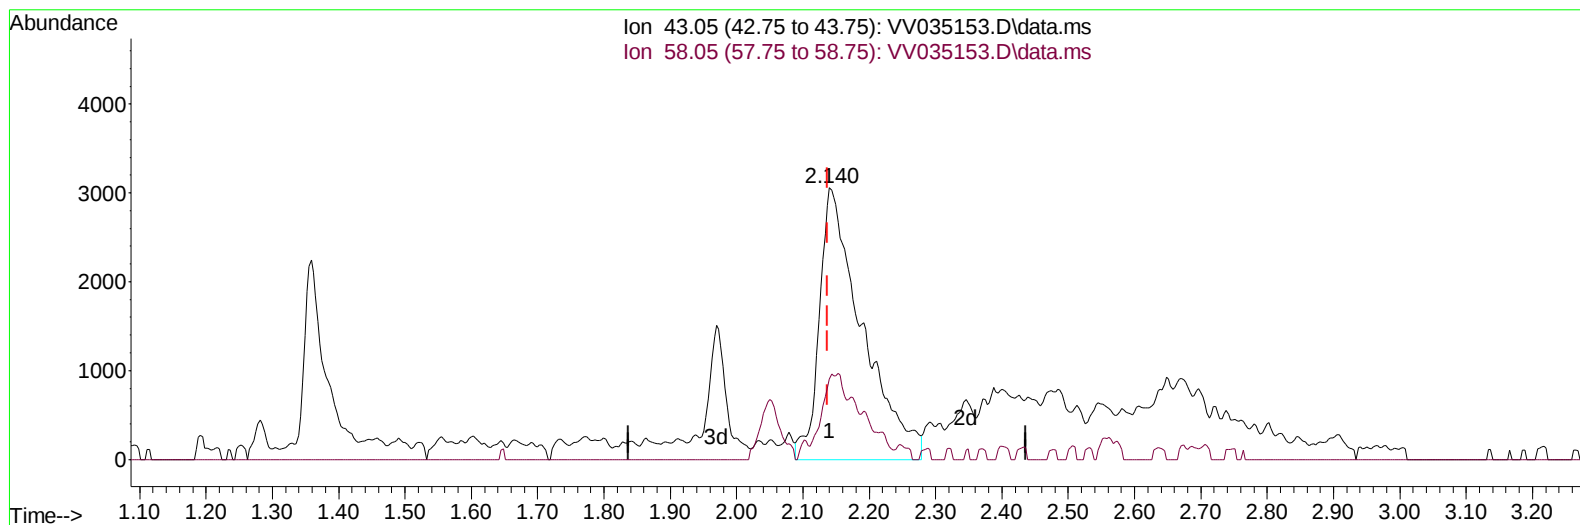

TIC: VV035153.D\data.ms

(13) Acetone (T)

2.140min (+ 0.003) 8.46 ug/L m

response 13652

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	12.79
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035153.D
 Acq On : 12 Apr 2024 03:42
 Operator : SY/MD
 Sample : P2057-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBM8

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:55:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:02:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
 Supervised By :Semsettin Yesilyurt 04/16/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		171517	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		174388	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		77619	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		55222	3.907	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.200%	
7) Chloroethane-d5	1.532	69		55839	4.791	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.800%	
11) 1,1-Dichloroethene-d2	2.060	65		27339	4.258	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.200%	
20) 2-Butanone-d5	3.818	46		154782	69.984	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	139.960%#	
24) Chloroform-d	4.249	84		119903	5.242	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%	
26) 1,2-Dichloroethane-d4	4.947	65		61141	5.919	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.400%	
32) Benzene-d6	4.960	84		228268	5.004	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%	
36) 1,2-Dichloropropane-d6	5.989	67		76696	5.728	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.600%	
41) Toluene-d8	7.246	98		183913	4.438	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%	
43) trans-1,3-Dichloroprop...	7.561	79		19748	4.152	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.000%	
46) 2-Hexanone-d5	8.027	63		110807	67.881	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	135.760%#	
56) 1,1,2,2-Tetrachloroeth...	10.153	84		56376	6.035	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	120.600%#	
66) 1,2-Dichlorobenzene-d4	11.561	152		67984	5.561	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.200%	
Target Compounds							
13) Acetone	2.140	43		13652m	8.462	ug/L	
47) Tetrachloroethene	7.902	164		340260	32.557	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035153.D
Acq On : 12 Apr 2024 03:42
Operator : SY/MD
Sample : P2057-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBM8

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:55:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:02:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

