




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035157.D
 Acq On : 12 Apr 2024 05:17
 Operator : SY/MD
 Sample : P2057-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:56:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:02:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
 Supervised By :Semsettin Yesilyurt 04/16/2024

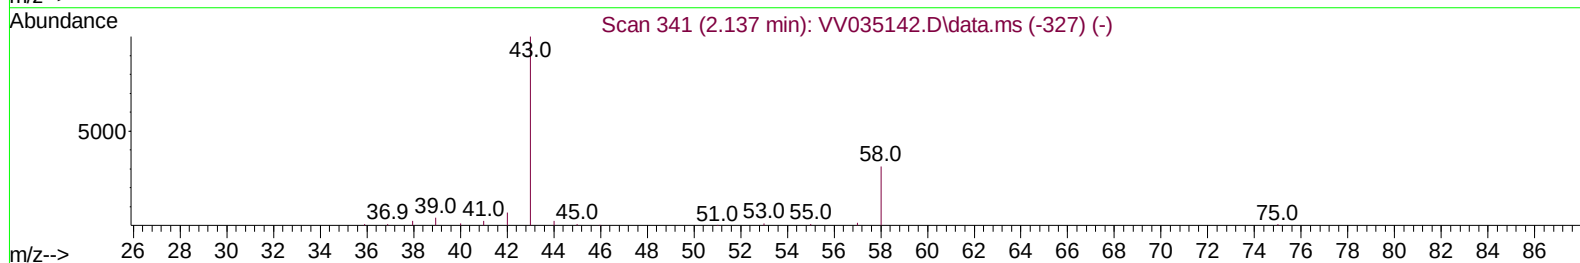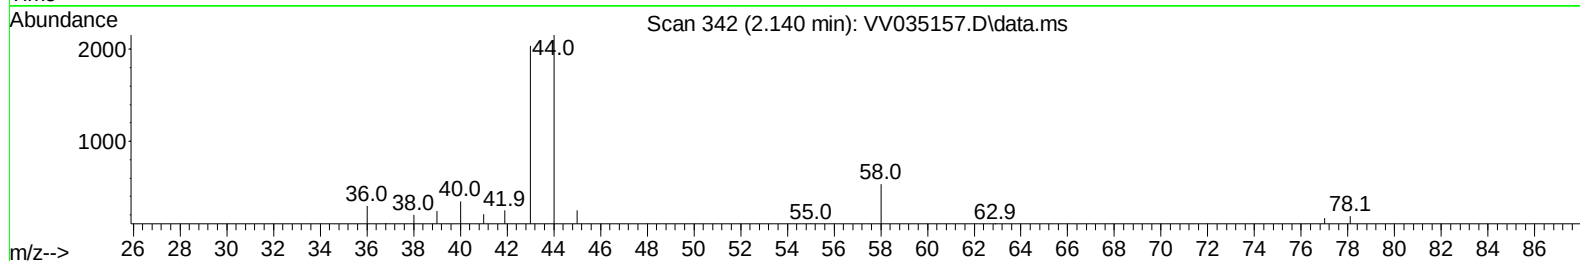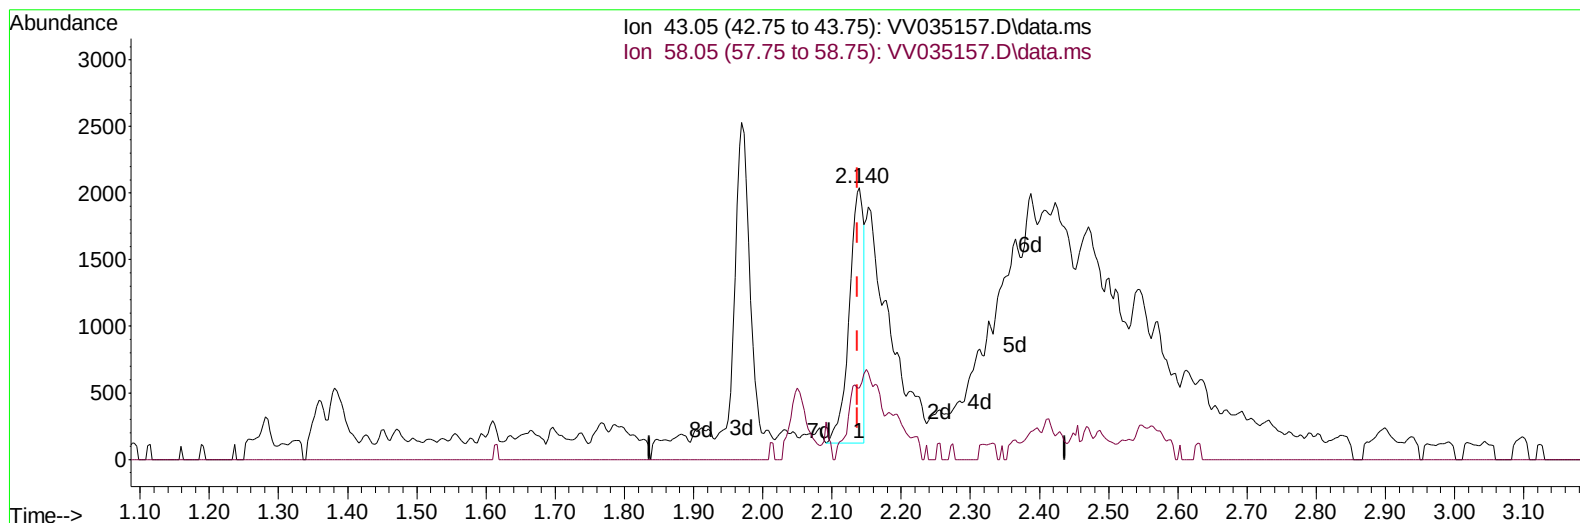

TIC: VV035157.D\data.ms

(13) Acetone (T)

2.140min (+ 0.003) 1.78 ug/L

response 2800

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	25.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035157.D
 Acq On : 12 Apr 2024 05:17
 Operator : SY/MD
 Sample : P2057-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBP1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:56:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:02:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
 Supervised By :Semsettin Yesilyurt 04/16/2024

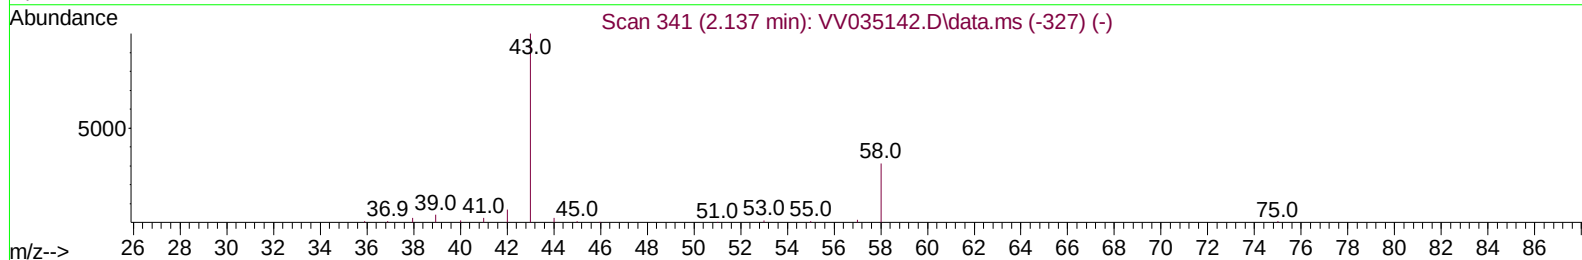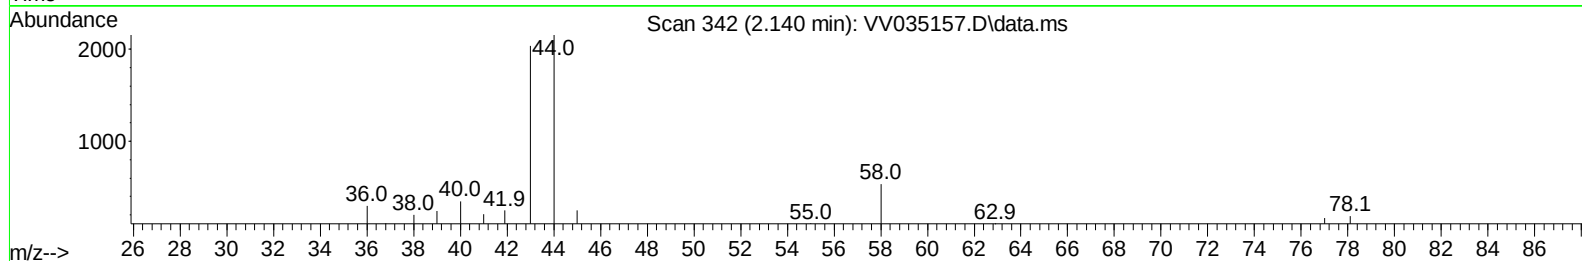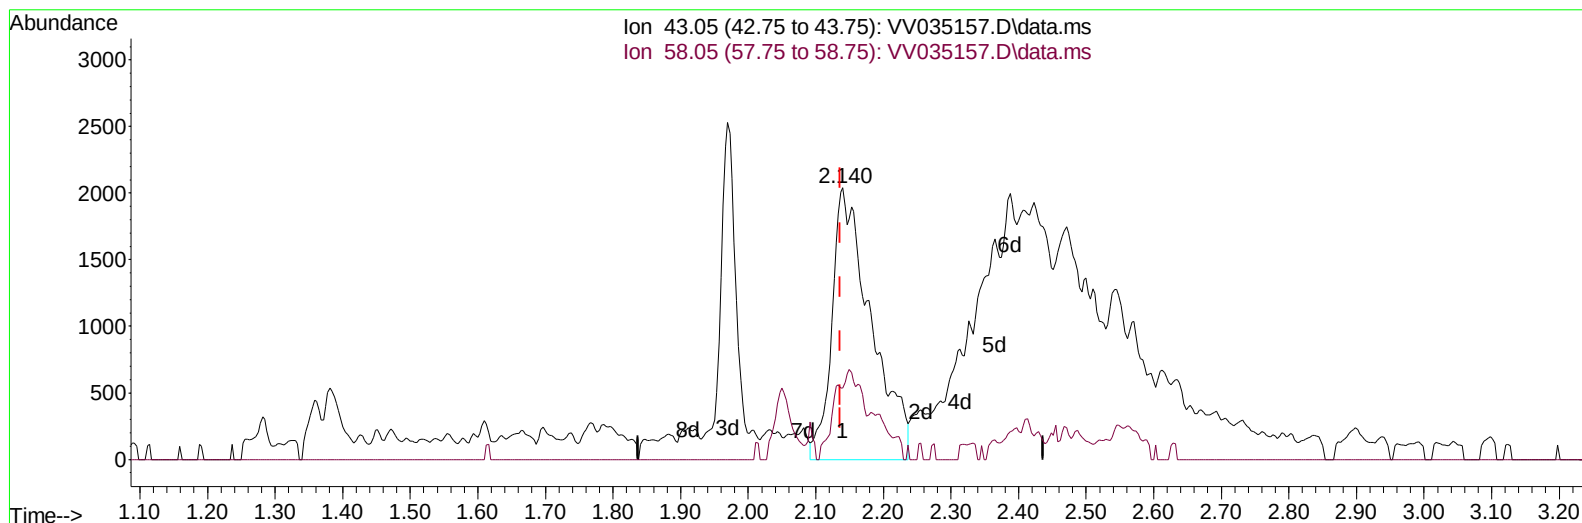

TIC: VV035157.D\data.ms

(13) Acetone (T)

2.140min (+ 0.003) 5.18 ug/L m

response 8146

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	8.77
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035157.D
 Acq On : 12 Apr 2024 05:17
 Operator : SY/MD
 Sample : P2057-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBP1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:56:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:02:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
 Supervised By :Semsettin Yesilyurt 04/16/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		167309	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		172601	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		75313	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		31491	2.284	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	45.600%	
7) Chloroethane-d5	1.532	69		29987	2.638	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	52.800%#	
11) 1,1-Dichloroethene-d2	2.059	65		16053	2.563	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	51.200%#	
20) 2-Butanone-d5	3.825	46		87959	40.771	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	81.540%	
24) Chloroform-d	4.252	84		71734	3.215	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	64.400%#	
26) 1,2-Dichloroethane-d4	4.947	65		35557	3.529	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	70.600%	
32) Benzene-d6	4.963	84		131450	2.911	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	58.200%#	
36) 1,2-Dichloropropane-d6	5.989	67		43896	3.313	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	66.200%	
41) Toluene-d8	7.246	98		102921	2.509	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	50.200%#	
43) trans-1,3-Dichloroprop...	7.567	79		10906	2.317	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	46.400%#	
46) 2-Hexanone-d5	8.030	63		66942	41.434	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	82.860%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		33514	3.625	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	72.400%	
66) 1,2-Dichlorobenzene-d4	11.561	152		39474	3.328	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	66.600%#	
Target Compounds							
13) Acetone	2.140	43		8146m	5.176	ug/L	
47) Tetrachloroethene	7.902	164		1332441	128.813	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035157.D
Acq On : 12 Apr 2024 05:17
Operator : SY/MD
Sample : P2057-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP1

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:56:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:02:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/13/2024
Supervised By :Semsettin Yesilyurt 04/16/2024

