

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035130.D
 Acq On : 11 Apr 2024 17:45
 Operator : SY/MD
 Sample : P2056-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP2

Quant Time: Apr 12 01:21:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	187183	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	182478	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	82073	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	59700	3.870	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.400%
7) Chloroethane-d5	1.532	69	58740	4.618	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.400%
11) 1,1-Dichloroethene-d2	2.056	65	29656	4.233	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.600%
20) 2-Butanone-d5	3.834	46	138785	57.499	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.000%
24) Chloroform-d	4.249	84	120328	4.821	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	4.947	65	61832	5.485	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.800%
32) Benzene-d6	4.960	84	233536	4.892	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	5.989	67	76747	5.478	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.600%
41) Toluene-d8	7.246	98	192595	4.442	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	7.564	79	21659	4.352	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.000%
46) 2-Hexanone-d5	8.030	63	106623	62.422	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	124.840%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	55451	5.673	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	68966	5.335	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.600%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.902	164	1741112	159.210	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035130.D
Acq On : 11 Apr 2024 17:45
Operator : SY/MD
Sample : P2056-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP2


Quant Time: Apr 12 01:21:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

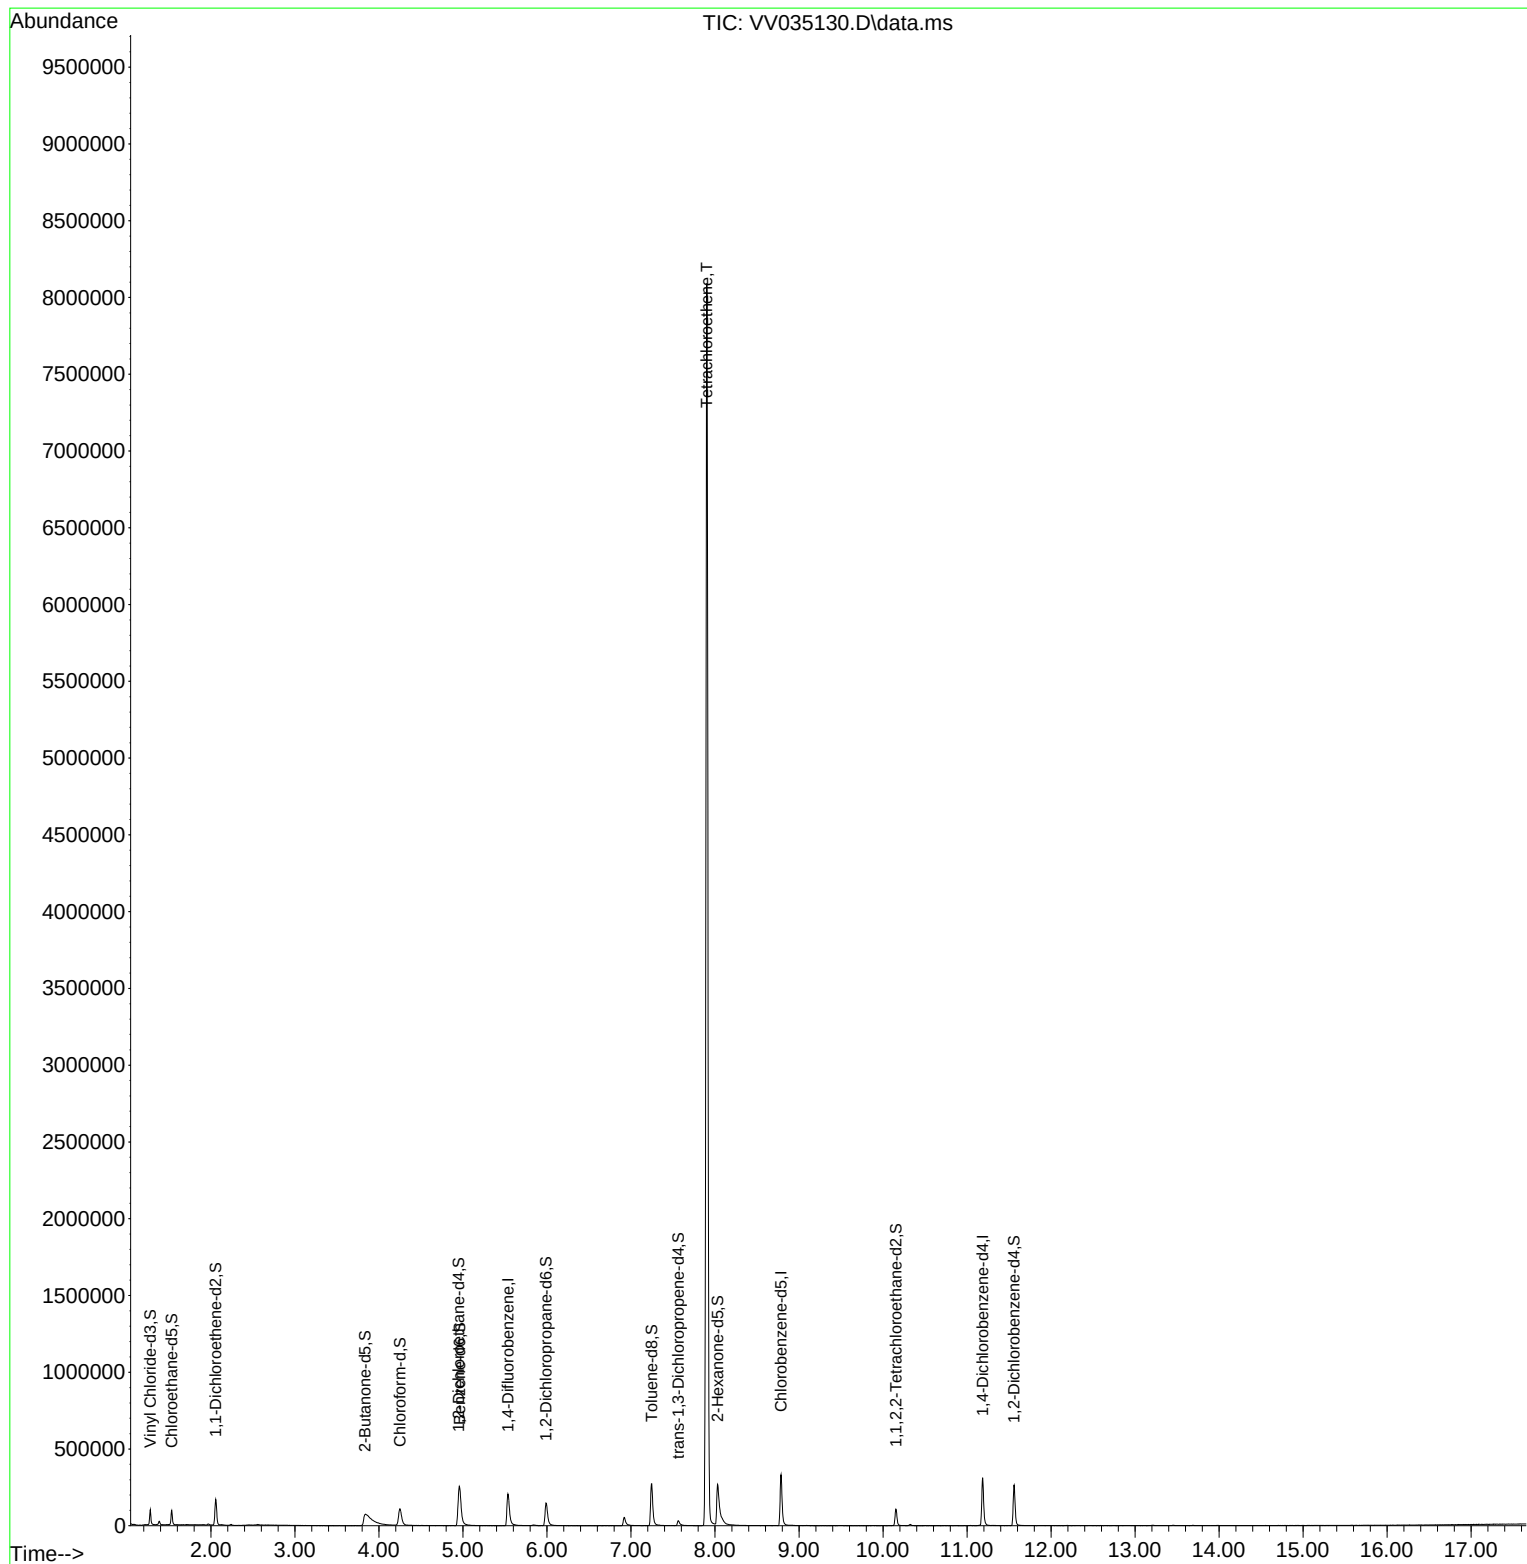

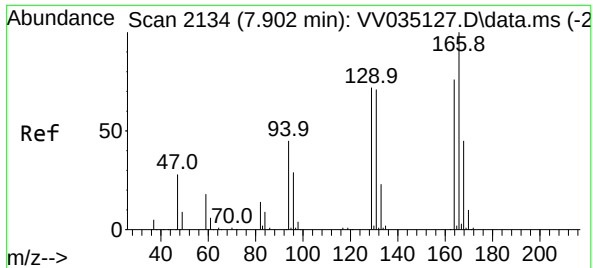

#47
 Tetrachloroethene
 Concen: 159.210 ug/L
 RT: 7.902 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VV035130.D
 Acq: 11 Apr 2024 17:45

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP2

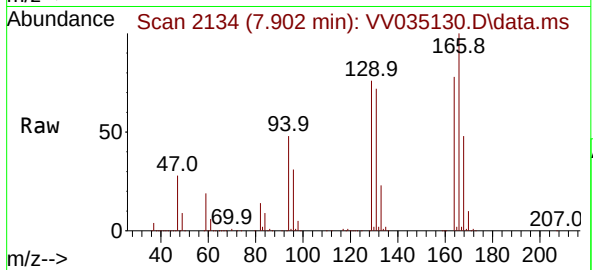

Tgt Ion:164 Resp: 1741112

Ion	Ratio	Lower	Upper
164	100		
129	96.5	66.0	122.6
131	91.9	63.0	117.0
166	127.4	91.9	170.7

