

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041124\
 Data File : VW035135.D
 Acq On : 11 Apr 2024 19:43
 Operator : SY/MD
 Sample : P2056-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP8

Quant Time: Apr 12 01:23:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	176966	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	182542	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.184	152	80426	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	57734	3.959	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.532	69	56660	4.712	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.200%
11) 1,1-Dichloroethene-d2	2.056	65	27093	4.090	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.800%
20) 2-Butanone-d5	3.831	46	141252	61.900	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.800%
24) Chloroform-d	4.252	84	116899	4.954	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	4.947	65	60925	5.717	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.400%
32) Benzene-d6	4.960	84	231311	4.844	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
36) 1,2-Dichloropropane-d6	5.989	67	76535	5.461	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.200%
41) Toluene-d8	7.246	98	185651	4.280	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%
43) trans-1,3-Dichloroprop...	7.561	79	21424	4.303	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.000%
46) 2-Hexanone-d5	8.030	63	98644	57.730	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	115.460%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	54678	5.592	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	67969	5.365	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.400%
Target Compounds						Qvalue
47) Tetrachloroethene	7.902	164	205090	18.747	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035135.D
Acq On : 11 Apr 2024 19:43
Operator : SY/MD
Sample : P2056-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP8


Quant Time: Apr 12 01:23:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

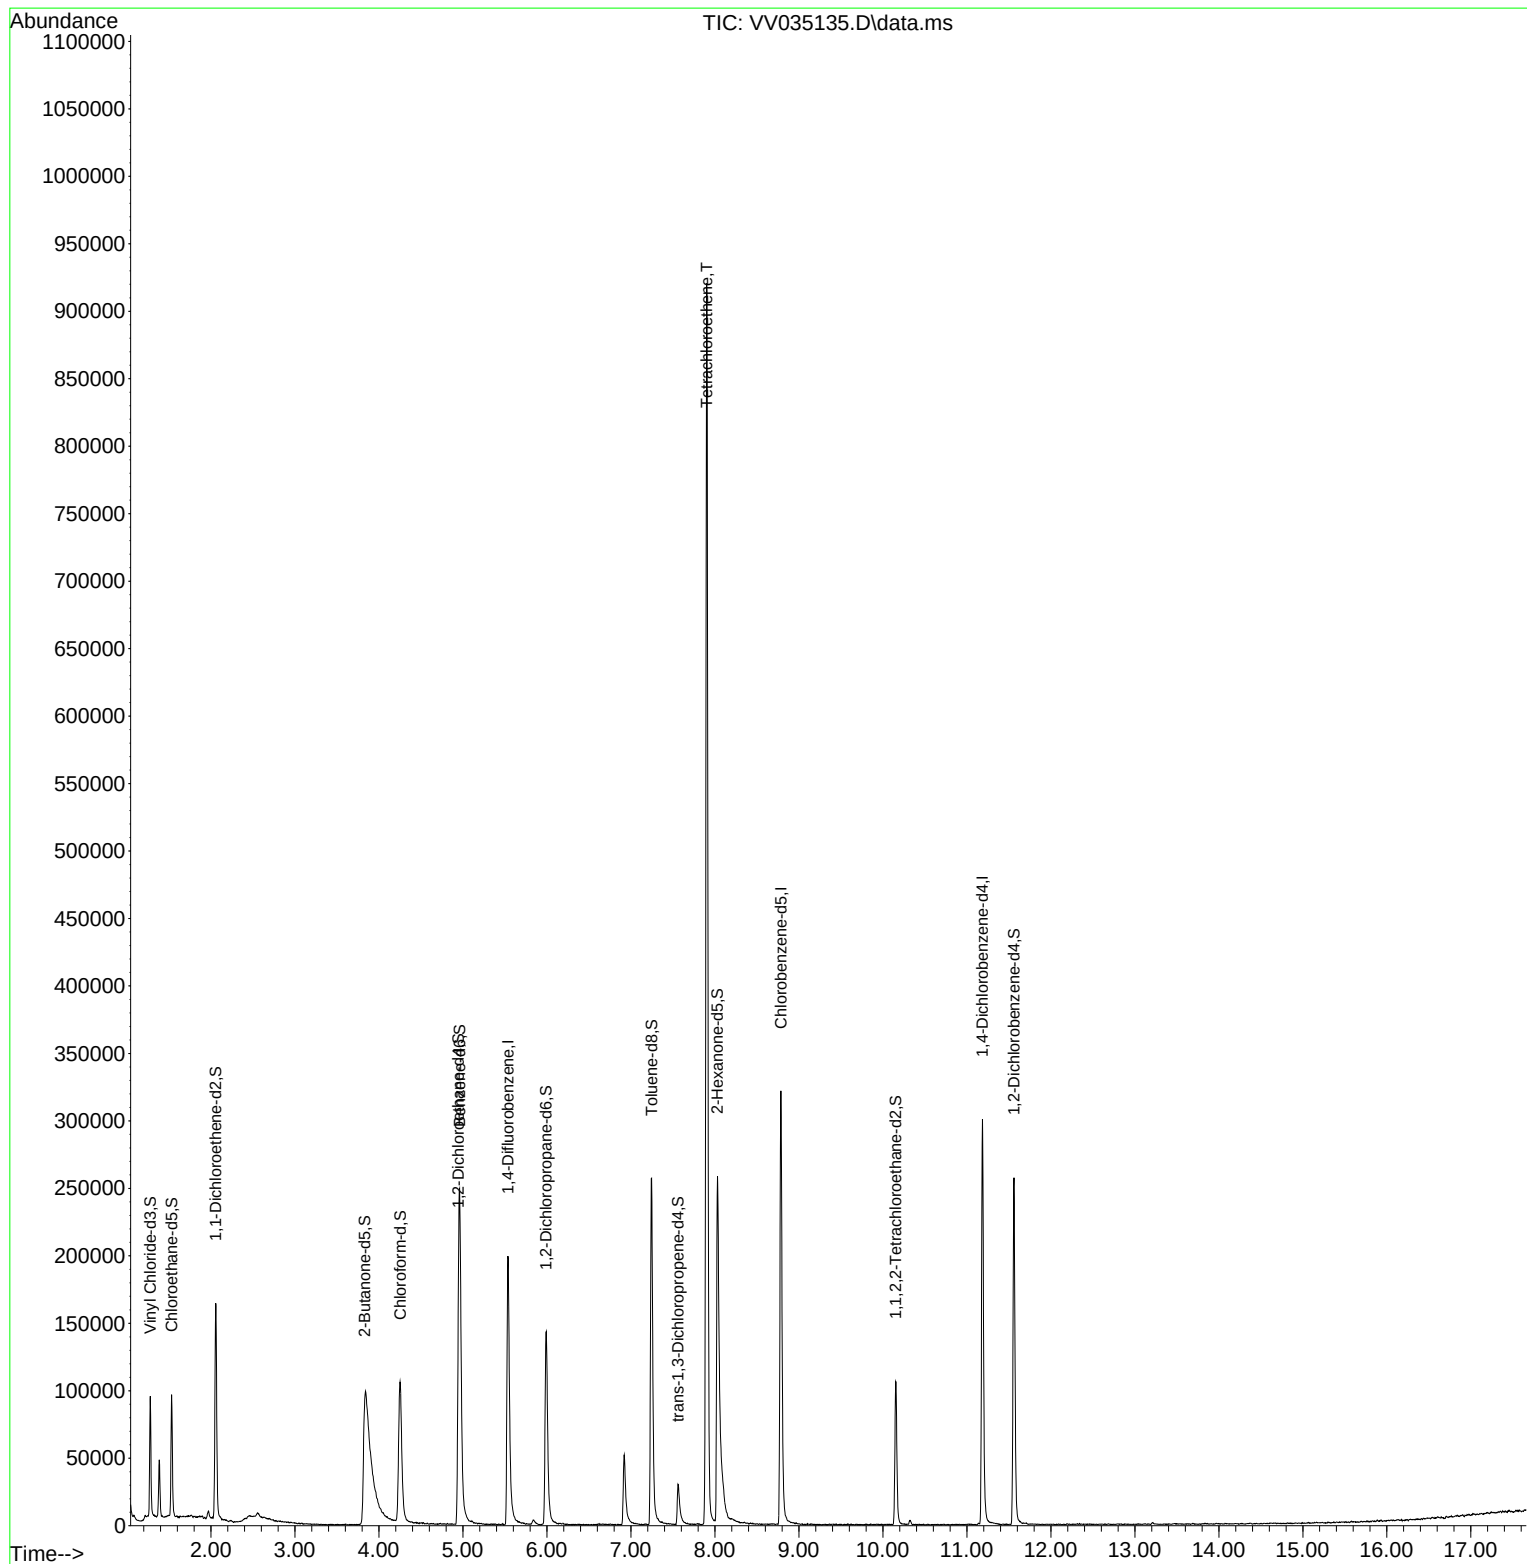

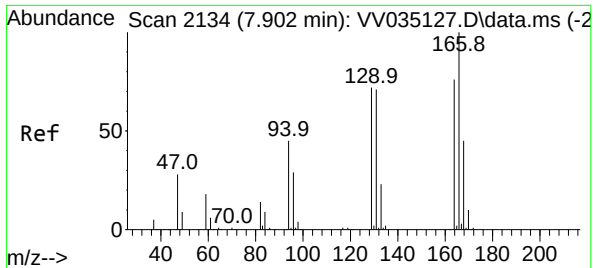

#47
 Tetrachloroethene
 Concen: 18.747 ug/L
 RT: 7.902 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VV035135.D
 Acq: 11 Apr 2024 19:43

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP8

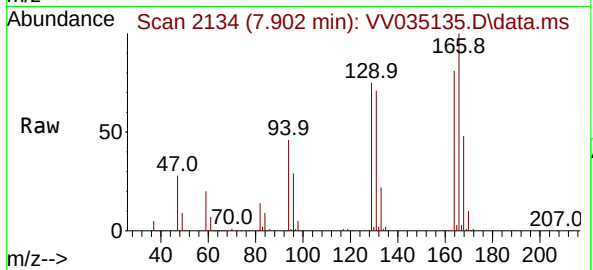

Tgt Ion:	164	Resp:	205090
Ion	Ratio	Lower	Upper
164	100		
129	93.7	66.0	122.6
131	88.5	63.0	117.0
166	124.2	91.9	170.7

