

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041124\
 Data File : VW035136.D
 Acq On : 11 Apr 2024 20:07
 Operator : SY/MD
 Sample : P2056-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ7

Quant Time: Apr 12 01:23:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	180107	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	181768	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	79265	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	58111	3.915	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.200%
7) Chloroethane-d5	1.532	69	57173	4.672	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.400%
11) 1,1-Dichloroethene-d2	2.056	65	28066	4.163	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.200%
20) 2-Butanone-d5	3.835	46	139554	60.089	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.180%
24) Chloroform-d	4.249	84	119817	4.989	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	4.944	65	61423	5.663	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.200%
32) Benzene-d6	4.960	84	236231	4.968	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
36) 1,2-Dichloropropane-d6	5.989	67	77410	5.547	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.000%
41) Toluene-d8	7.246	98	185765	4.301	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
43) trans-1,3-Dichloroprop...	7.561	79	21408	4.318	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.400%
46) 2-Hexanone-d5	8.031	63	94044	55.273	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.540%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	54959	5.644	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	112.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	67237	5.385	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%
Target Compounds						Qvalue
47) Tetrachloroethene	7.912	164	1952	0.179	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035136.D
Acq On : 11 Apr 2024 20:07
Operator : SY/MD
Sample : P2056-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ7


Quant Time: Apr 12 01:23:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

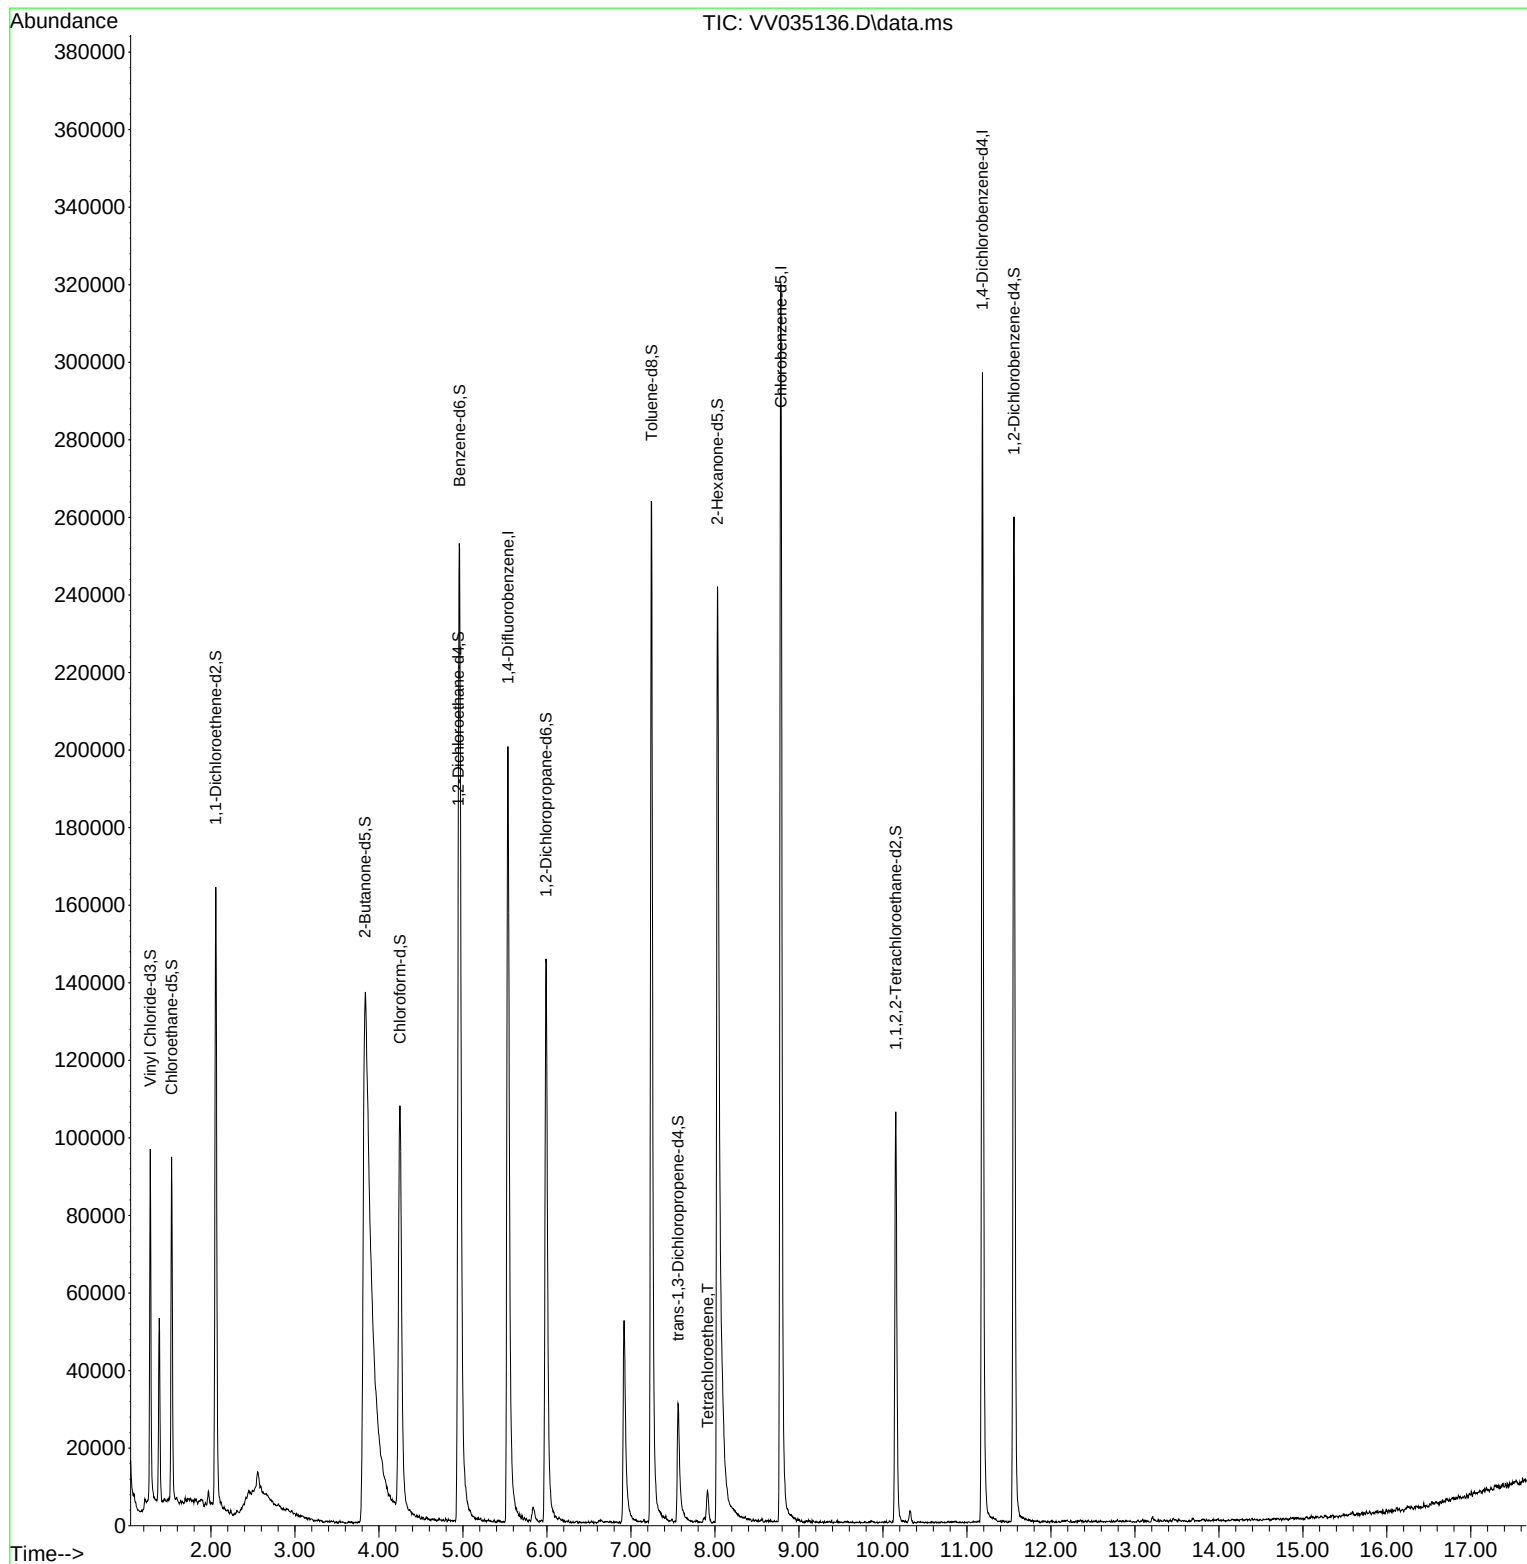

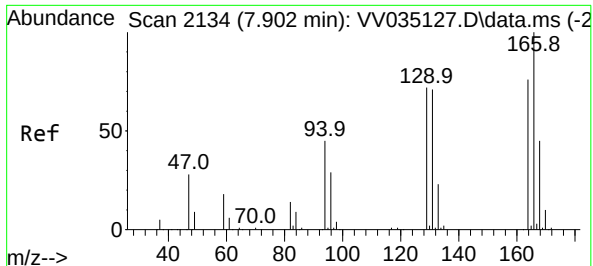

#47
 Tetrachloroethene
 Concen: 0.179 ug/L
 RT: 7.912 min Scan# 21
 Delta R.T. 0.010 min
 Lab File: VV035136.D
 Acq: 11 Apr 2024 20:07

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ7

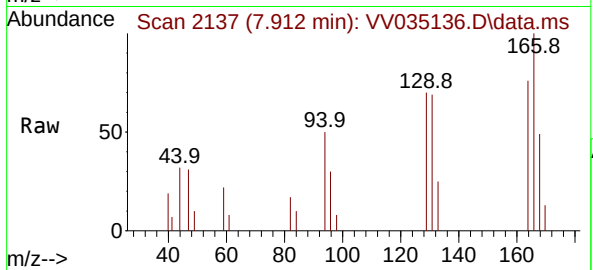

Tgt Ion:164 Resp: 1952

Ion	Ratio	Lower	Upper
164	100		
129	91.6	66.0	122.6
131	90.4	63.0	117.0
166	131.5	91.9	170.7

