

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041124\
 Data File : VW035137.D
 Acq On : 11 Apr 2024 20:30
 Operator : SY/MD
 Sample : P2056-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ9

Quant Time: Apr 12 01:23:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	181776	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	184805	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	79161	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	54961	3.669	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.400%
7) Chloroethane-d5	1.532	69	54541	4.416	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.400%
11) 1,1-Dichloroethene-d2	2.056	65	26858	3.947	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.000%
20) 2-Butanone-d5	3.831	46	122411	52.224	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.440%
24) Chloroform-d	4.249	84	113274	4.673	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
26) 1,2-Dichloroethane-d4	4.947	65	59268	5.414	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.200%
32) Benzene-d6	4.960	84	222388	4.600	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.000%
36) 1,2-Dichloropropane-d6	5.989	67	72762	5.128	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.600%
41) Toluene-d8	7.243	98	181259	4.128	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	7.561	79	20171	4.002	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	8.030	63	94857	54.834	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.660%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	53288	5.383	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.600%
66) 1,2-Dichlorobenzene-d4	11.561	152	65292	5.236	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.800%
Target Compounds						Qvalue
47) Tetrachloroethene	7.902	164	249193	22.500	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035137.D
Acq On : 11 Apr 2024 20:30
Operator : SY/MD
Sample : P2056-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ9


Quant Time: Apr 12 01:23:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

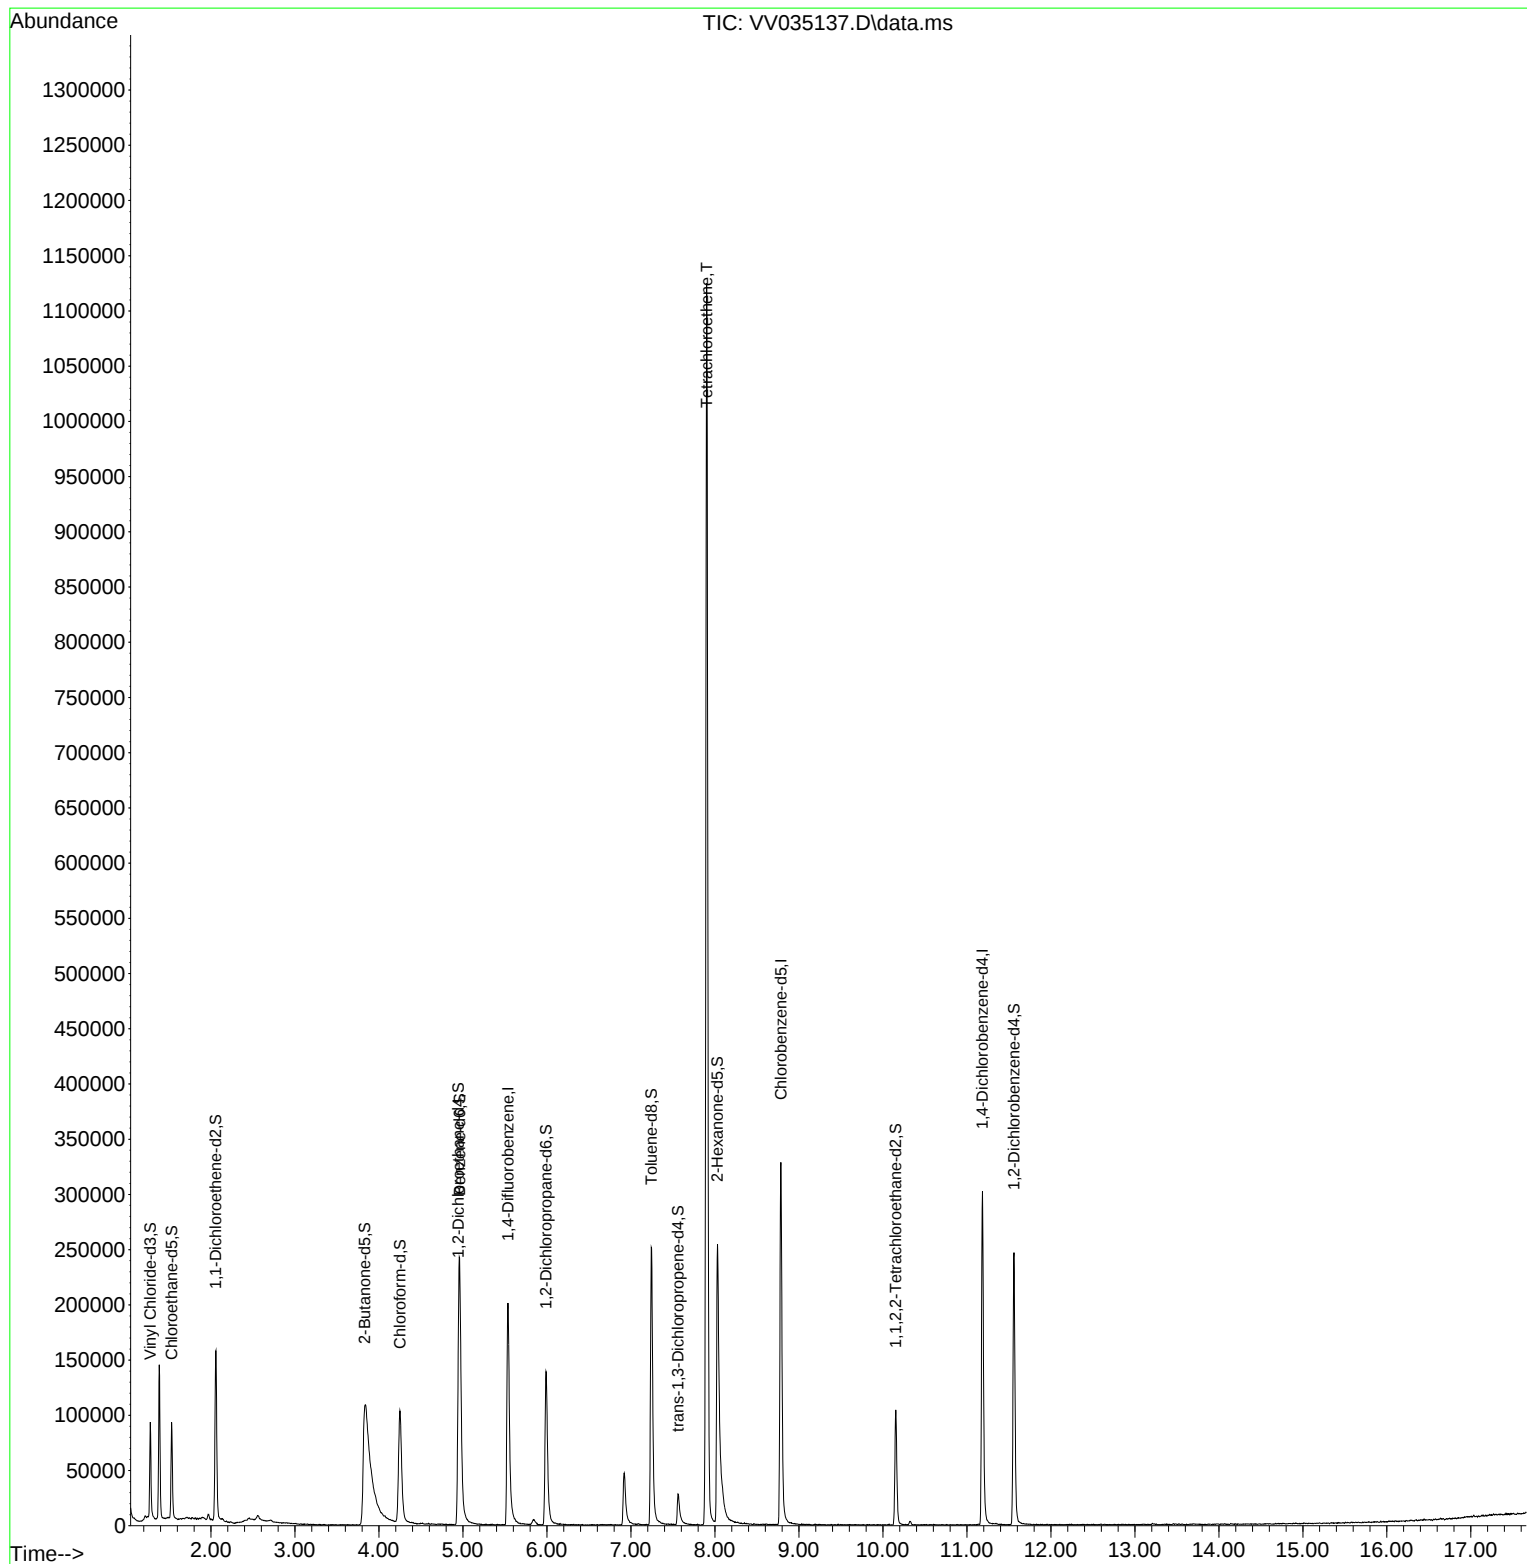

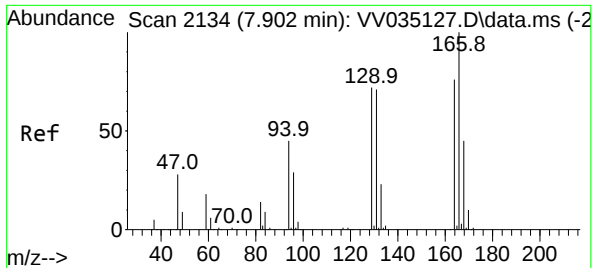

#47
 Tetrachloroethene
 Concen: 22.500 ug/L
 RT: 7.902 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VV035137.D
 Acq: 11 Apr 2024 20:30

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ9

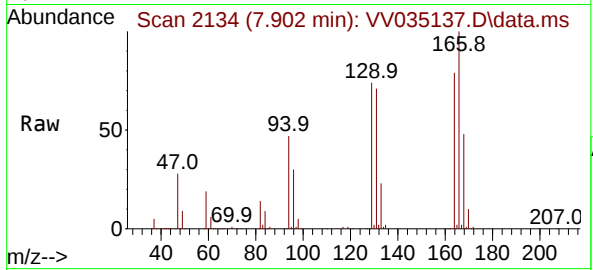

Tgt Ion:	164	Resp:	249193
Ion	Ratio	Lower	Upper
164	100		
129	93.3	66.0	122.6
131	89.7	63.0	117.0
166	126.5	91.9	170.7

