

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041124\
 Data File : VW035138.D
 Acq On : 11 Apr 2024 20:54
 Operator : SY/MD
 Sample : P2056-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BS4

Quant Time: Apr 12 01:23:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 01:20:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	152531	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	156938	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	67610	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	55839	4.442	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.800%	
7) Chloroethane-d5	1.532	69	54518	5.260	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	105.200%	
11) 1,1-Dichloroethene-d2	2.060	65	27400	4.799	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	96.000%	
20) 2-Butanone-d5	3.831	46	144721	73.580	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	147.160%#	
24) Chloroform-d	4.249	84	114727	5.640	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	112.800%	
26) 1,2-Dichloroethane-d4	4.944	65	60294	6.564	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	131.200%#	
32) Benzene-d6	4.960	84	217947	5.309	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	106.200%	
36) 1,2-Dichloropropane-d6	5.989	67	72706	6.034	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	120.600%	
41) Toluene-d8	7.243	98	175551	4.708	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.200%	
43) trans-1,3-Dichloroprop...	7.561	79	20318	4.747	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.000%	
46) 2-Hexanone-d5	8.031	63	107122	72.920	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	145.840%#	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	56405	6.709	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	134.200%#	
66) 1,2-Dichlorobenzene-d4	11.561	152	64168	6.025	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	120.600%#	
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.902	164	253273	26.929	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035138.D
Acq On : 11 Apr 2024 20:54
Operator : SY/MD
Sample : P2056-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BS4


Quant Time: Apr 12 01:23:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 01:20:53 2024
Response via : Initial Calibration

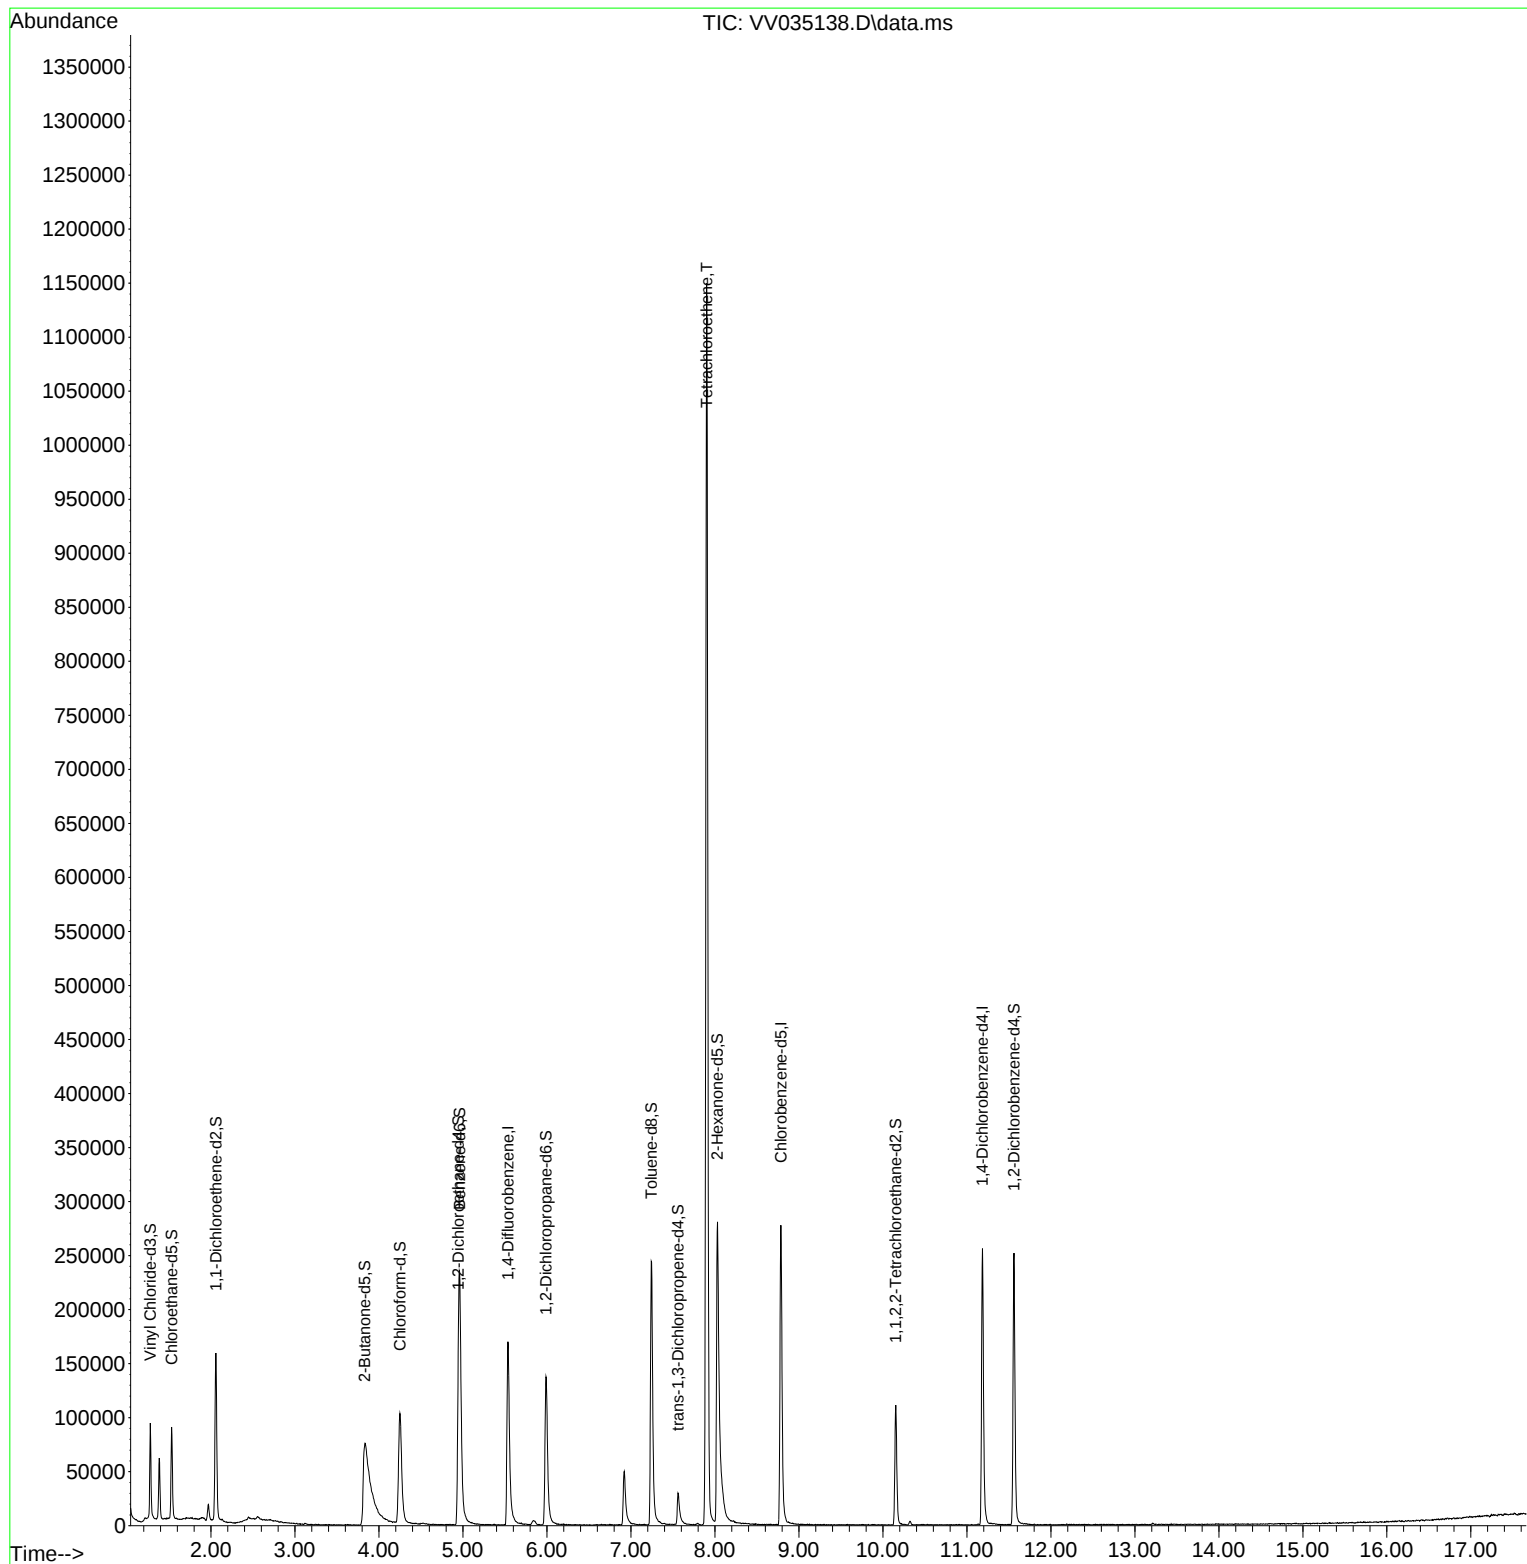

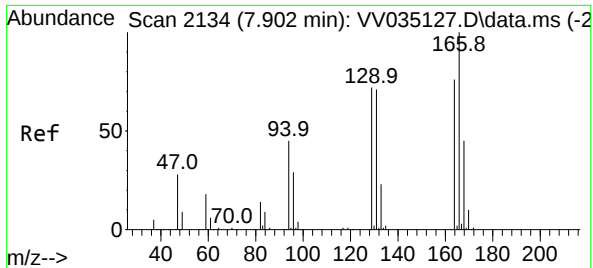

#47
 Tetrachloroethene
 Concen: 26.929 ug/L
 RT: 7.902 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VV035138.D
 Acq: 11 Apr 2024 20:54

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BS4

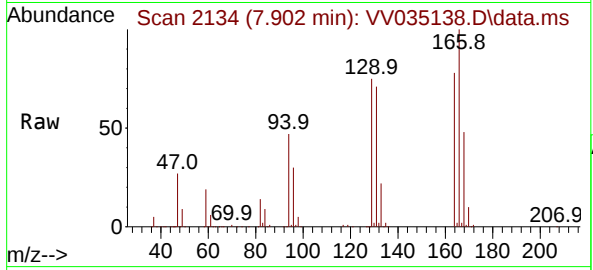

Tgt Ion:164 Resp: 253273

Ion	Ratio	Lower	Upper
164	100		
129	95.9	66.0	122.6
131	91.1	63.0	117.0
166	128.7	91.9	170.7

