

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041124\
 Data File : VW035144.D
 Acq On : 12 Apr 2024 00:06
 Operator : SY/MD
 Sample : P2057-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBL1

Quant Time: Apr 12 02:07:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:02:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	176758	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	178312	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	75833	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	59630	4.093	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.800%
7) Chloroethane-d5	1.529	69	59004	4.913	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.200%
11) 1,1-Dichloroethene-d2	2.057	65	28895	4.367	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.400%
20) 2-Butanone-d5	3.831	46	124892	54.795	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.600%
24) Chloroform-d	4.249	84	125683	5.332	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.600%
26) 1,2-Dichloroethane-d4	4.944	65	63279	5.945	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.800%
32) Benzene-d6	4.960	84	238554	5.114	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.200%
36) 1,2-Dichloropropane-d6	5.989	67	78177	5.710	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.200%
41) Toluene-d8	7.243	98	192381	4.540	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.800%
43) trans-1,3-Dichloroprop...	7.561	79	19916	4.095	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.000%
46) 2-Hexanone-d5	8.031	63	103166	61.809	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.620%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	58534	6.128	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	122.600%#
66) 1,2-Dichlorobenzene-d4	11.561	152	67606	5.660	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.200%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.908	164	7647	0.716	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035144.D
Acq On : 12 Apr 2024 00:06
Operator : SY/MD
Sample : P2057-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBL1


Quant Time: Apr 12 02:07:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:02:37 2024
Response via : Initial Calibration

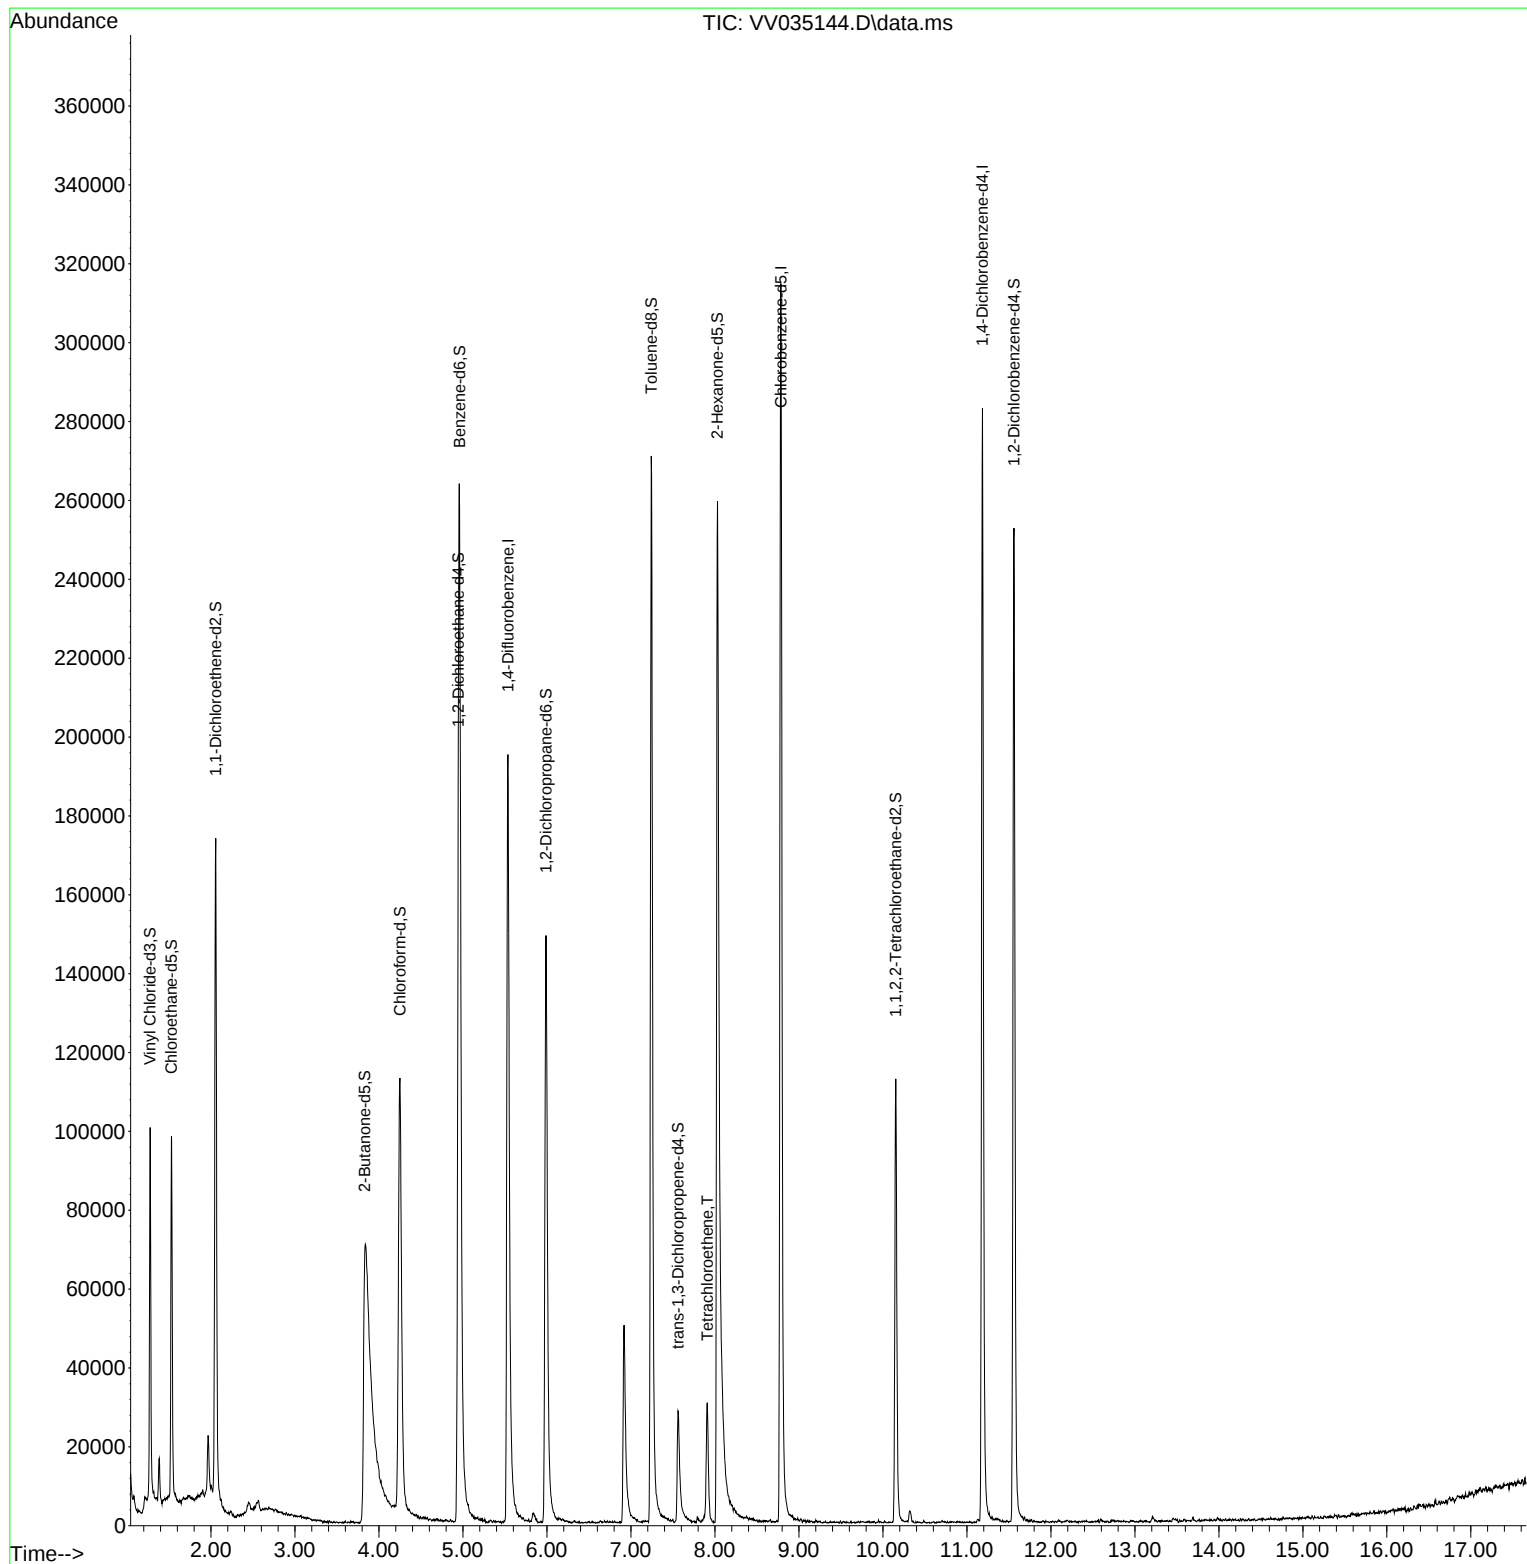

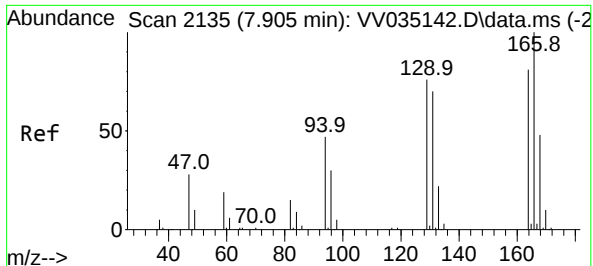

#47
 Tetrachloroethene
 Concen: 0.716 ug/L
 RT: 7.908 min Scan# 2136
 Delta R.T. 0.003 min
 Lab File: VV035144.D
 Acq: 12 Apr 2024 00:06

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BL1

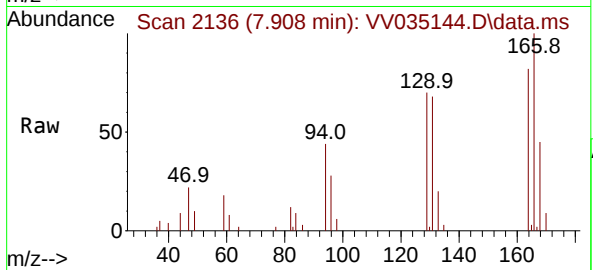

Tgt Ion:	164	Resp:	7647
Ion	Ratio	Lower	Upper
164	100		
129	85.6	66.0	122.6
131	83.2	63.0	117.0
166	121.6	91.9	170.7

