

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041124\
 Data File : VW035149.D
 Acq On : 12 Apr 2024 02:06
 Operator : SY/MD
 Sample : P2057-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBL7

Quant Time: Apr 12 05:54:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:02:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	171887	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	178231	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	77467	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	54712	3.862	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.200%	
7) Chloroethane-d5	1.532	69	55262	4.732	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.600%	
11) 1,1-Dichloroethene-d2	2.060	65	25673	3.990	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	79.800%	
20) 2-Butanone-d5	3.815	46	152417	68.766	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	137.540%#	
24) Chloroform-d	4.249	84	119342	5.207	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.200%	
26) 1,2-Dichloroethane-d4	4.944	65	62202	6.009	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	120.200%	
32) Benzene-d6	4.960	84	229311	4.918	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.400%	
36) 1,2-Dichloropropane-d6	5.989	67	76343	5.579	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	111.600%	
41) Toluene-d8	7.243	98	181333	4.282	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	7.561	79	19562	4.024	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	80.400%	
46) 2-Hexanone-d5	8.027	63	119385	71.559	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	143.120%#	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	57209	5.992	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	119.800%	
66) 1,2-Dichlorobenzene-d4	11.561	152	67526	5.534	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.600%	
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.905	164	2030428	190.090	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035149.D
Acq On : 12 Apr 2024 02:06
Operator : SY/MD
Sample : P2057-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBL7


Quant Time: Apr 12 05:54:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:02:37 2024
Response via : Initial Calibration

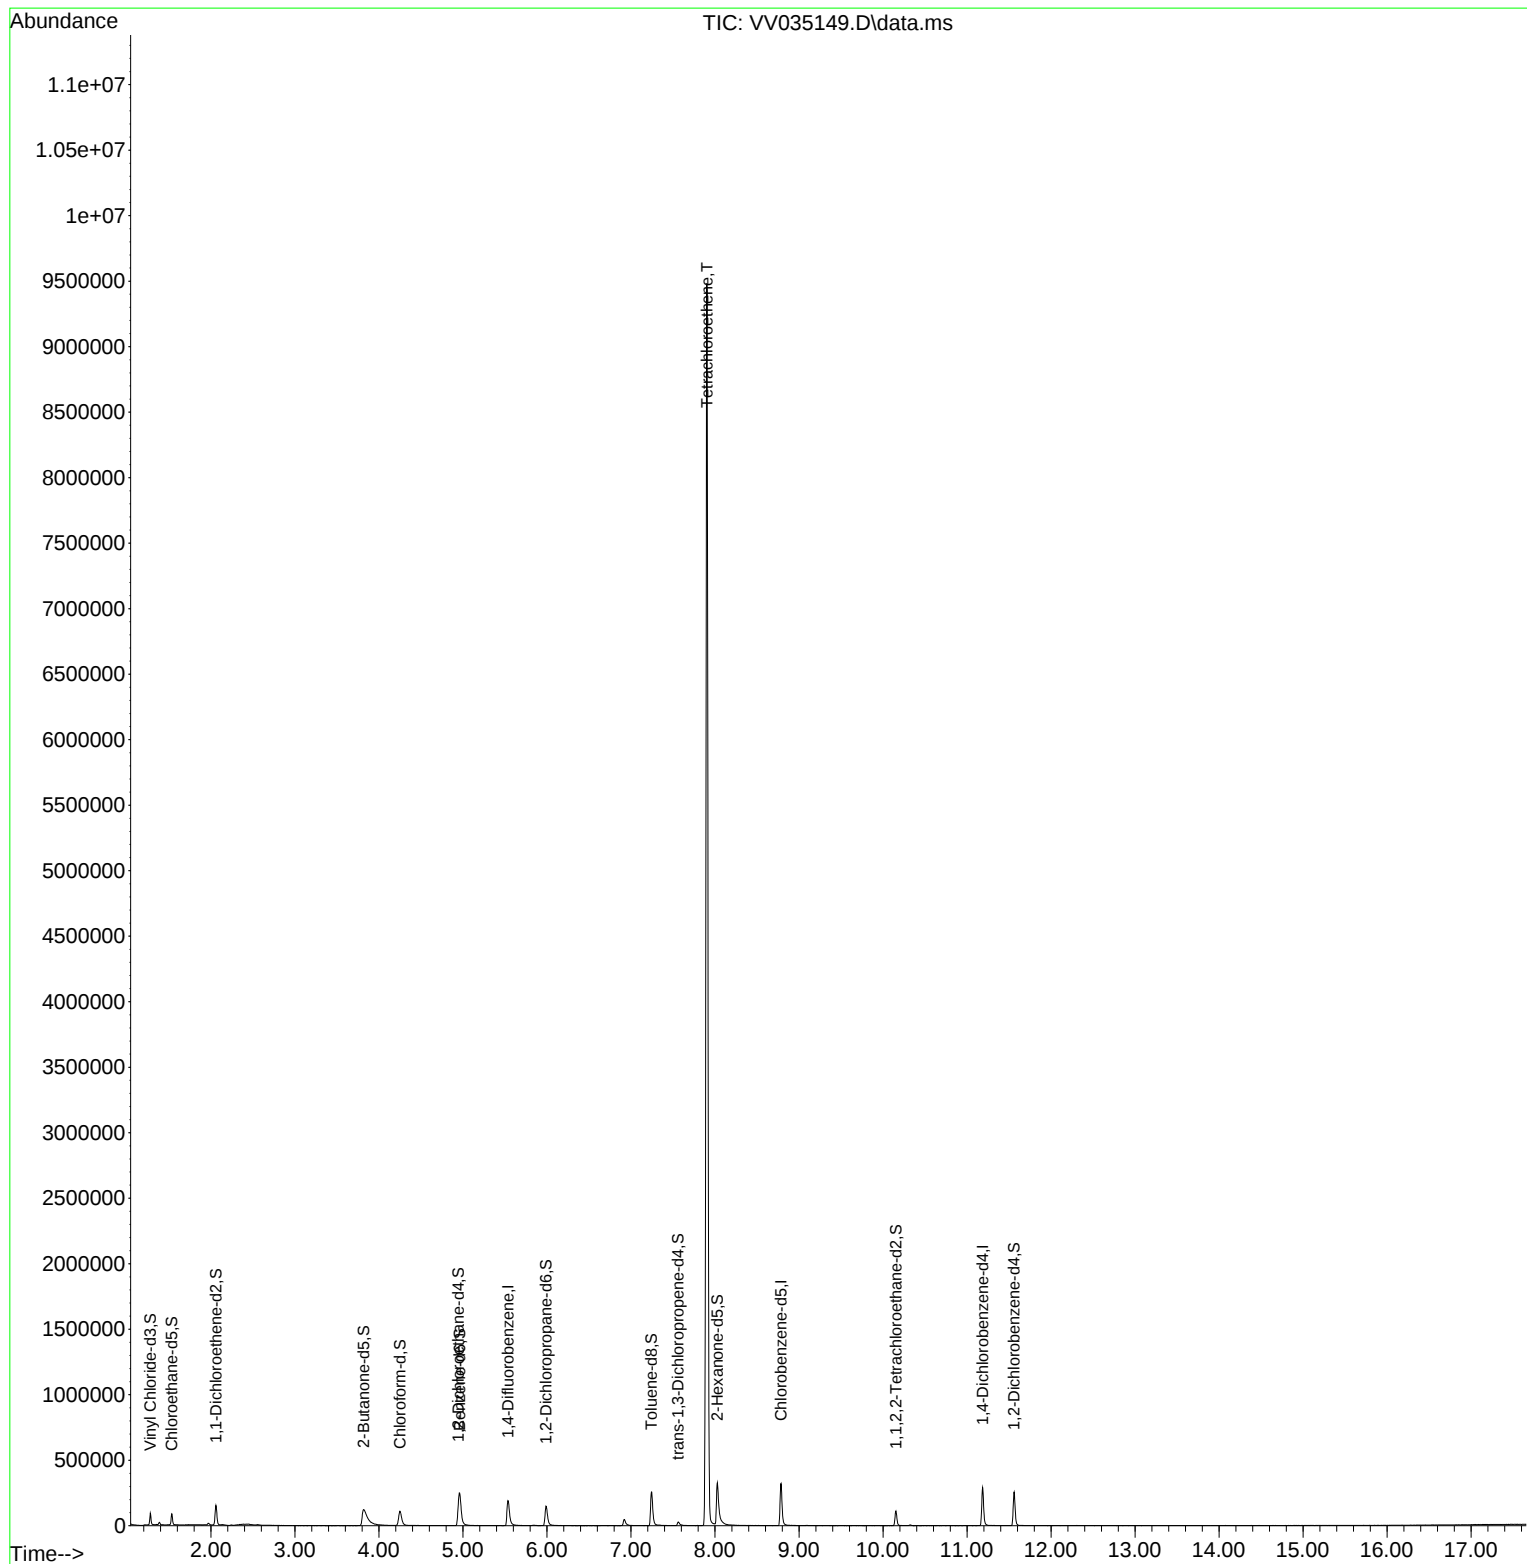

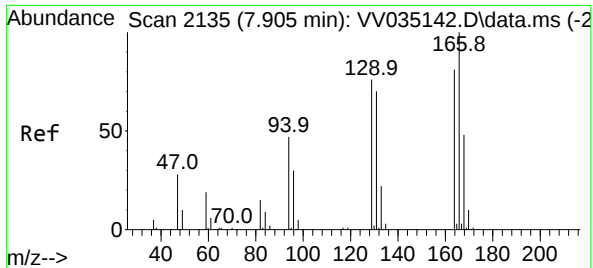

#47
 Tetrachloroethene
 Concen: 190.090 ug/L
 RT: 7.905 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VV035149.D
 Acq: 12 Apr 2024 02:06

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BL7

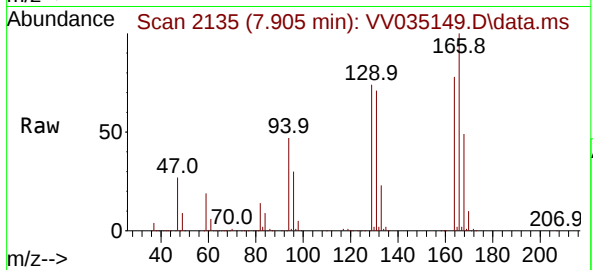

Tgt Ion:164 Resp: 2030428

Ion	Ratio	Lower	Upper
164	100		
129	95.0	66.0	122.6
131	91.5	63.0	117.0
166	128.2	91.9	170.7

