

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041124\
 Data File : VW035155.D
 Acq On : 12 Apr 2024 04:30
 Operator : SY/MD
 Sample : P2057-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBN3

Quant Time: Apr 12 05:56:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:02:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	172017	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	176190	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	75433	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	29186	2.059	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	41.200%
7) Chloroethane-d5	1.532	69	29270	2.504	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	50.000%#
11) 1,1-Dichloroethene-d2	2.060	65	15729	2.443	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	48.800%#
20) 2-Butanone-d5	3.825	46	79940	36.040	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.080%
24) Chloroform-d	4.249	84	69305	3.021	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	60.400%#
26) 1,2-Dichloroethane-d4	4.947	65	32321	3.120	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	62.400%#
32) Benzene-d6	4.963	84	126228	2.739	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	54.800%#
36) 1,2-Dichloropropane-d6	5.992	67	43429	3.211	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	64.200%
41) Toluene-d8	7.246	98	98108	2.343	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	46.800%#
43) trans-1,3-Dichloroprop...	7.567	79	11548	2.403	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	48.000%#
46) 2-Hexanone-d5	8.030	63	56208	34.081	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.160%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	32575	3.451	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	69.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	38460	3.237	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	64.800%#
Target Compounds						Qvalue
47) Tetrachloroethene	7.905	164	27278	2.583	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035155.D
Acq On : 12 Apr 2024 04:30
Operator : SY/MD
Sample : P2057-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBN3


Quant Time: Apr 12 05:56:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:02:37 2024
Response via : Initial Calibration

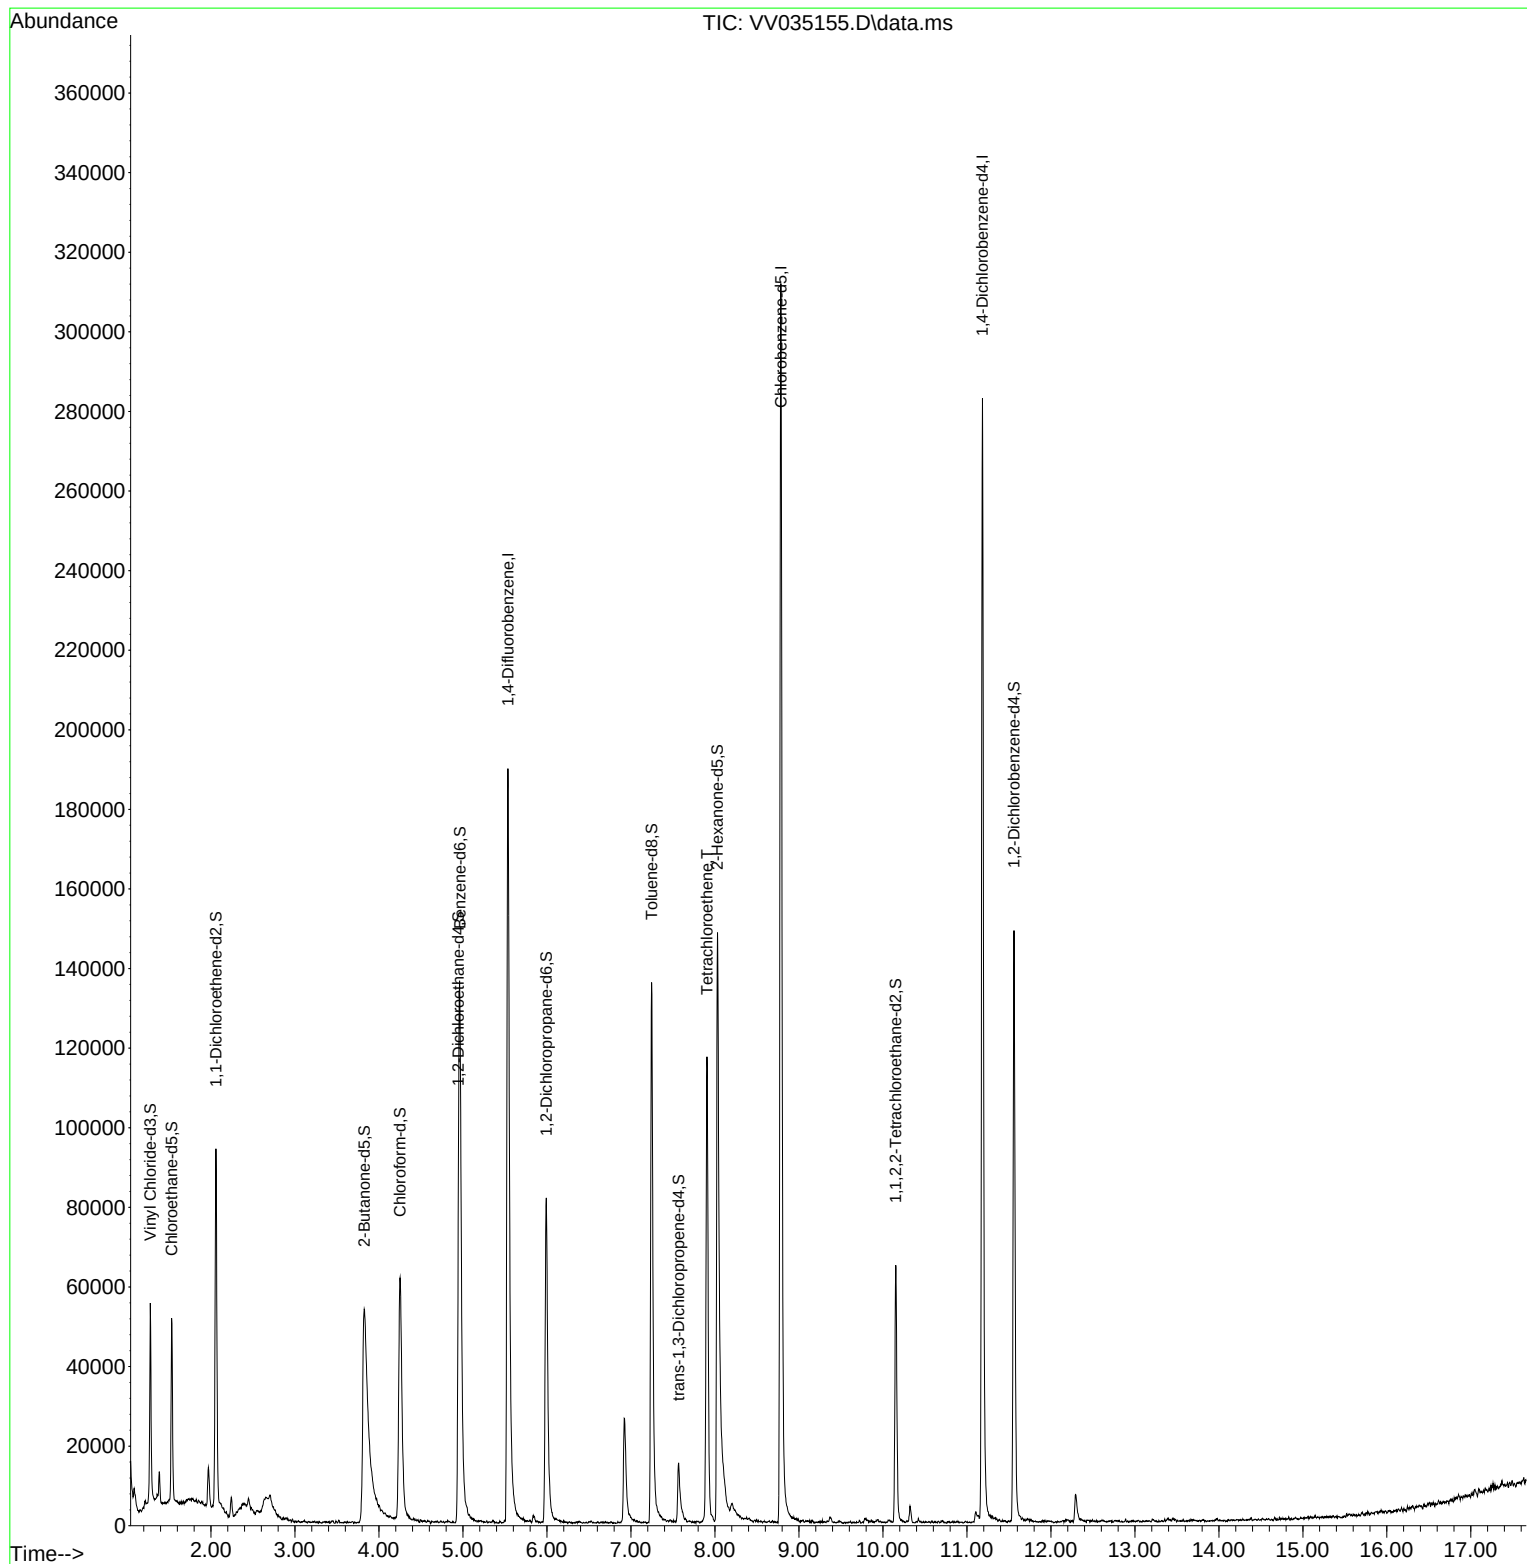

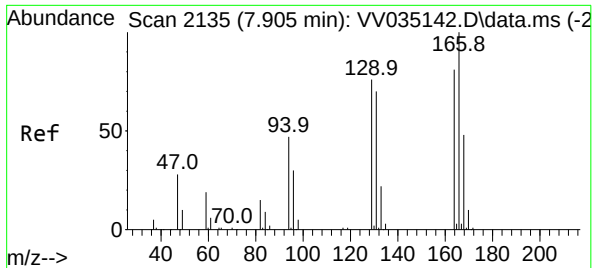

#47
 Tetrachloroethene
 Concen: 2.583 ug/L
 RT: 7.905 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VV035155.D
 Acq: 12 Apr 2024 04:30

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BN3

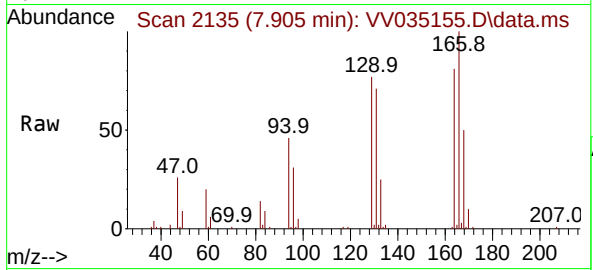

Tgt Ion:	164	Resp:	27278
Ion	Ratio	Lower	Upper
164	100		
129	95.8	66.0	122.6
131	87.9	63.0	117.0
166	123.7	91.9	170.7

