

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035158.D
 Acq On : 12 Apr 2024 05:41
 Operator : SY/MD
 Sample : P2057-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP3

Quant Time: Apr 12 06:29:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:02:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	176420	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	180494	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	79181	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	53892	3.707	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.200%
7) Chloroethane-d5	1.532	69	54378	4.536	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.800%
11) 1,1-Dichloroethene-d2	2.060	65	25463	3.856	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.200%
20) 2-Butanone-d5	3.815	46	151421	66.562	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	133.120%#
24) Chloroform-d	4.249	84	117396	4.990	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	4.944	65	59934	5.641	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.800%
32) Benzene-d6	4.960	84	222068	4.703	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	5.989	67	75047	5.416	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.400%
41) Toluene-d8	7.246	98	175210	4.085	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.800%
43) trans-1,3-Dichloroprop...	7.561	79	18152	3.687	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.800%
46) 2-Hexanone-d5	8.027	63	101135	59.860	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.720%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	55524	5.743	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	65820	5.277	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.600%
Target Compounds						Qvalue
47) Tetrachloroethene	7.905	164	10885	1.006	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035158.D
Acq On : 12 Apr 2024 05:41
Operator : SY/MD
Sample : P2057-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP3


Quant Time: Apr 12 06:29:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:02:37 2024
Response via : Initial Calibration

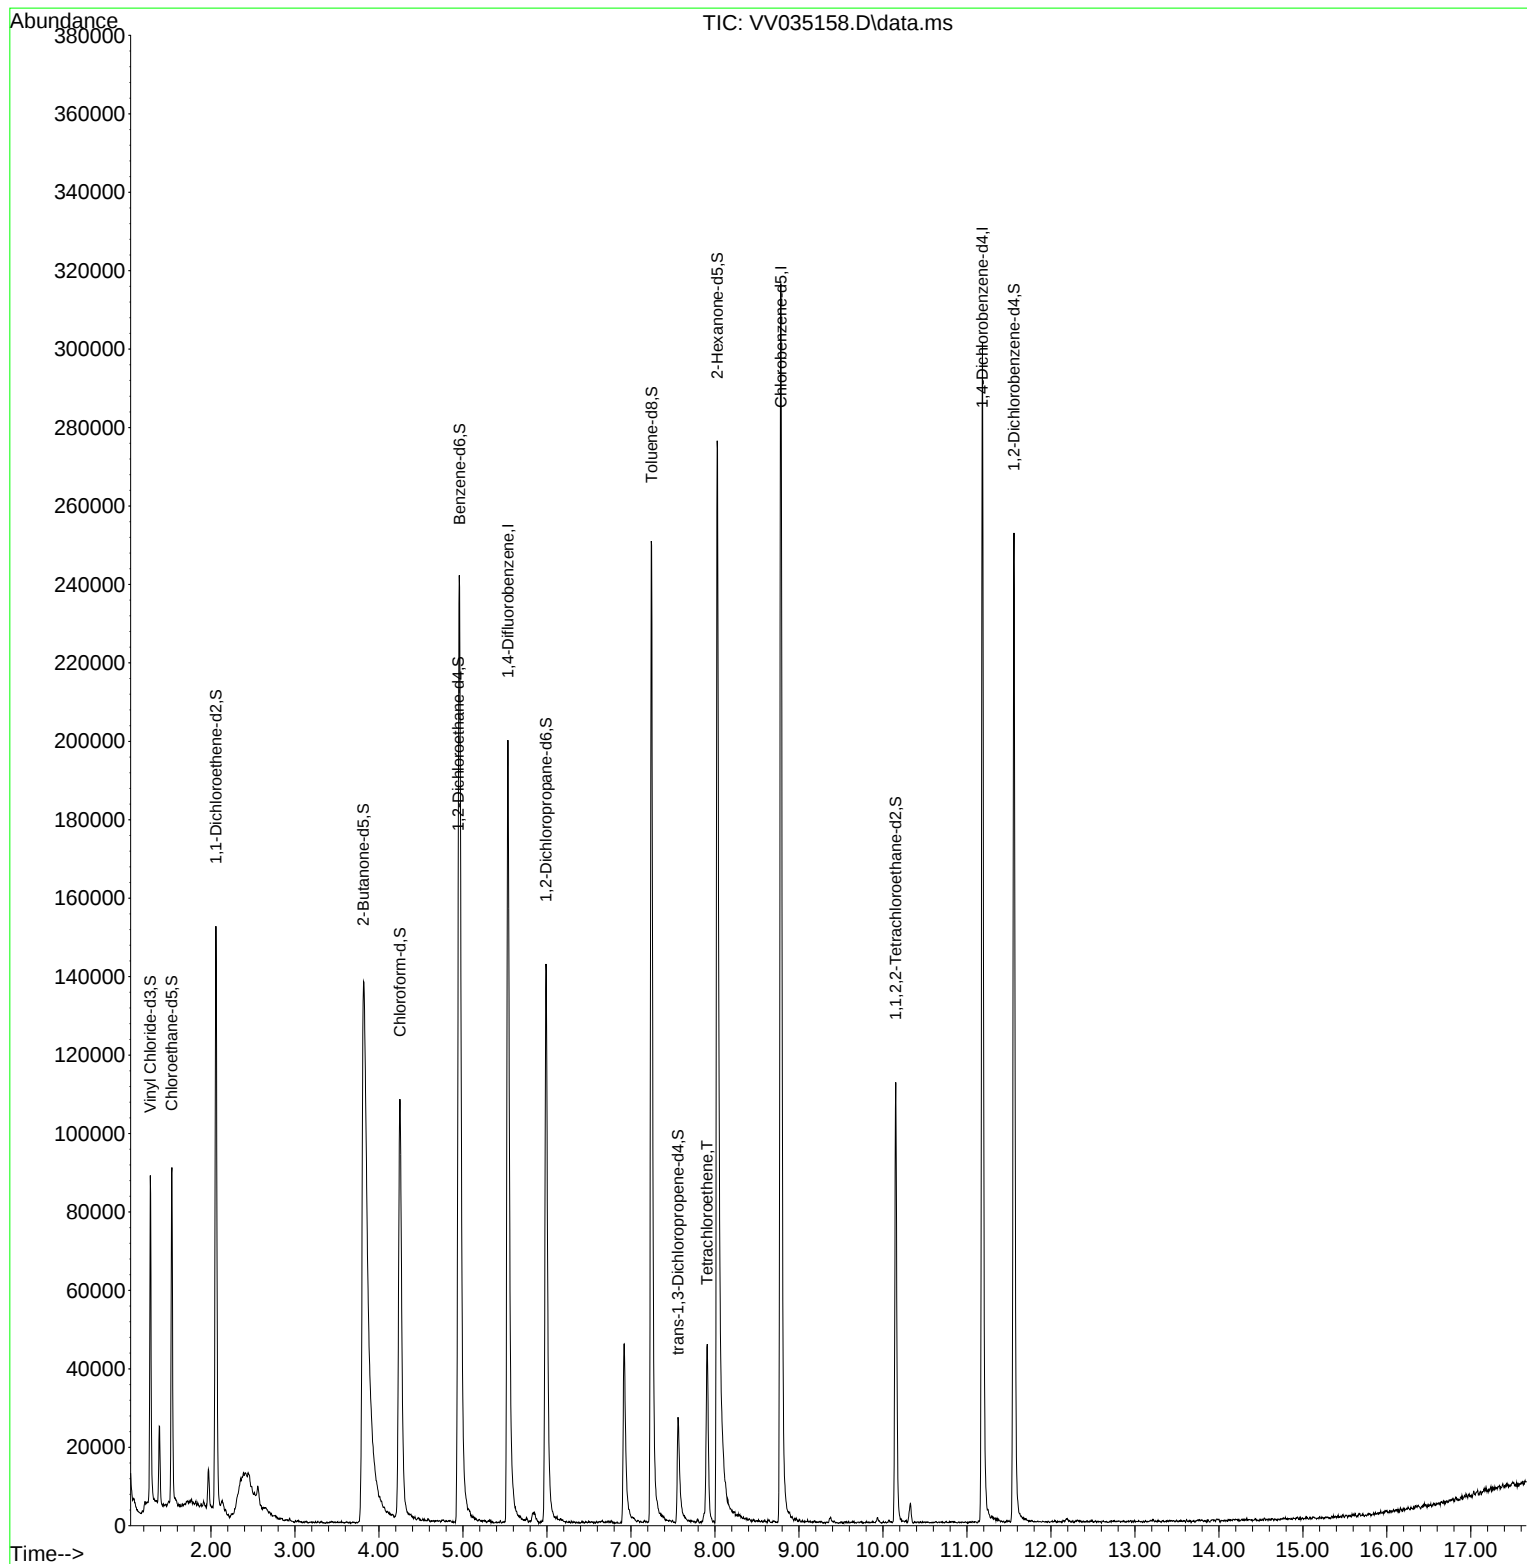

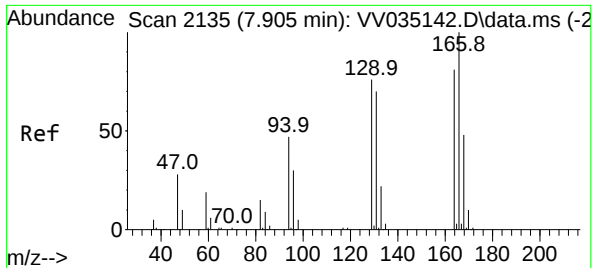

#47
 Tetrachloroethene
 Concen: 1.006 ug/L
 RT: 7.905 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VV035158.D
 Acq: 12 Apr 2024 05:41

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP3

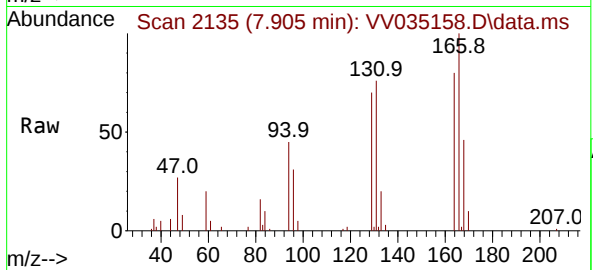

Tgt Ion:	164	Resp:	10885
Ion	Ratio	Lower	Upper
164	100		
129	87.1	66.0	122.6
131	94.6	63.0	117.0
166	124.9	91.9	170.7

