

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035128.D
 Acq On : 11 Apr 2024 16:54
 Operator : SY/MD
 Sample : VV0411WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	88660	93872	14.78%	1.827%
2	1.532	145	153	168	rBV	89124	106707	16.80%	2.077%
3	2.060	306	317	334	rBV	154189	225505	35.50%	4.389%
4	2.449	428	438	453	rVB4	6739	13153	2.07%	0.256%
5	3.812	853	862	901	rBV	36324	148694	23.41%	2.894%
6	4.246	983	997	1023	rVB2	103621	270661	42.61%	5.268%
7	4.957	1203	1218	1254	rBV2	244854	635241	100.00%	12.365%
8	5.535	1387	1398	1428	rBV	202550	440819	69.39%	8.580%
9	5.838	1481	1492	1505	rBV9	3742	9243	1.46%	0.180%
10	5.989	1524	1539	1567	rBV	144438	310524	48.88%	6.044%
11	6.918	1818	1828	1848	rBV	50871	108978	17.16%	2.121%
12	7.243	1919	1929	1955	rBV	262249	481578	75.81%	9.374%
13	7.561	2019	2028	2047	rBV2	28500	60856	9.58%	1.185%
14	8.031	2163	2174	2231	rBV2	186794	574053	90.37%	11.174%
15	8.783	2397	2408	2438	rBV	322927	561898	88.45%	10.937%
16	10.153	2820	2834	2856	rBV	99905	169130	26.62%	3.292%
17	11.185	3145	3155	3178	rBV	303646	496504	78.16%	9.664%
18	11.561	3260	3272	3299	rBV	254450	423522	66.67%	8.244%
19	13.452	3850	3860	3870	rBV4	4017	6676	1.05%	0.130%




Sum of corrected areas: 5137614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035128.D
Acq On : 11 Apr 2024 16:54
Operator : SY/MD
Sample : VV0411WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

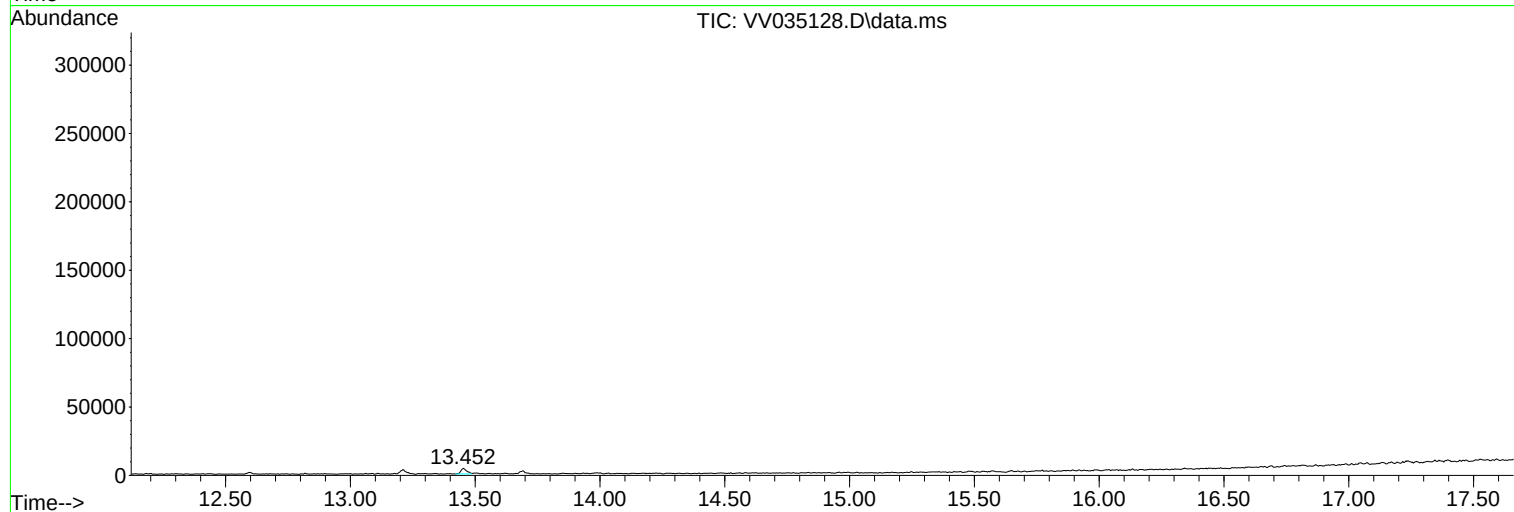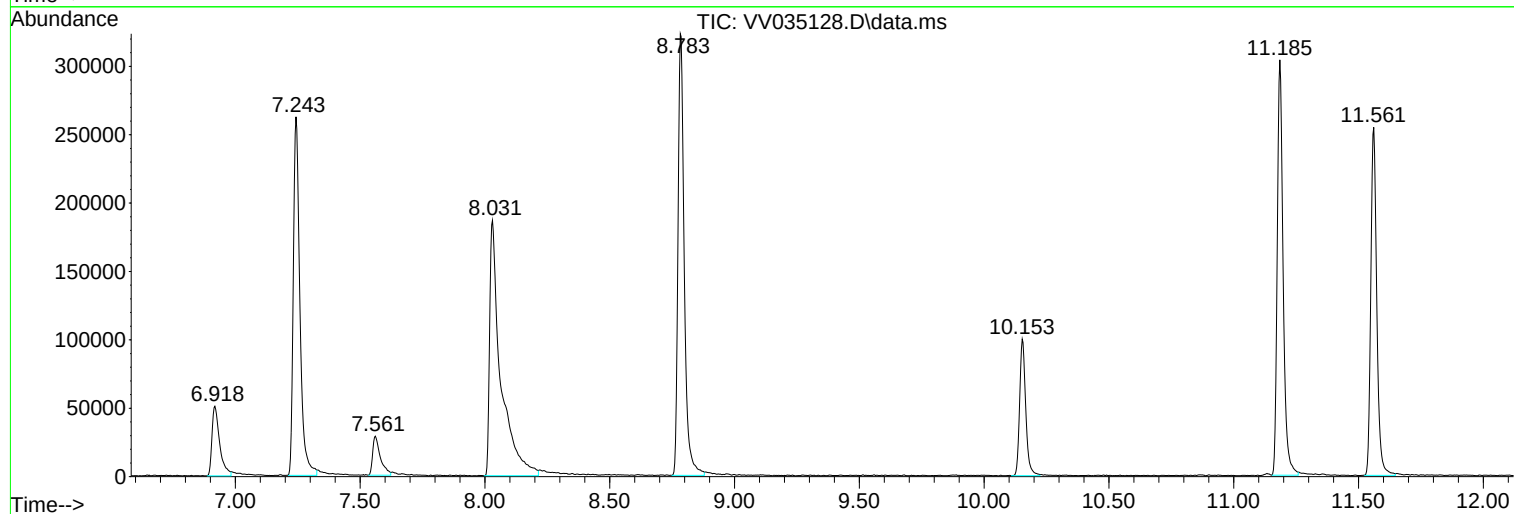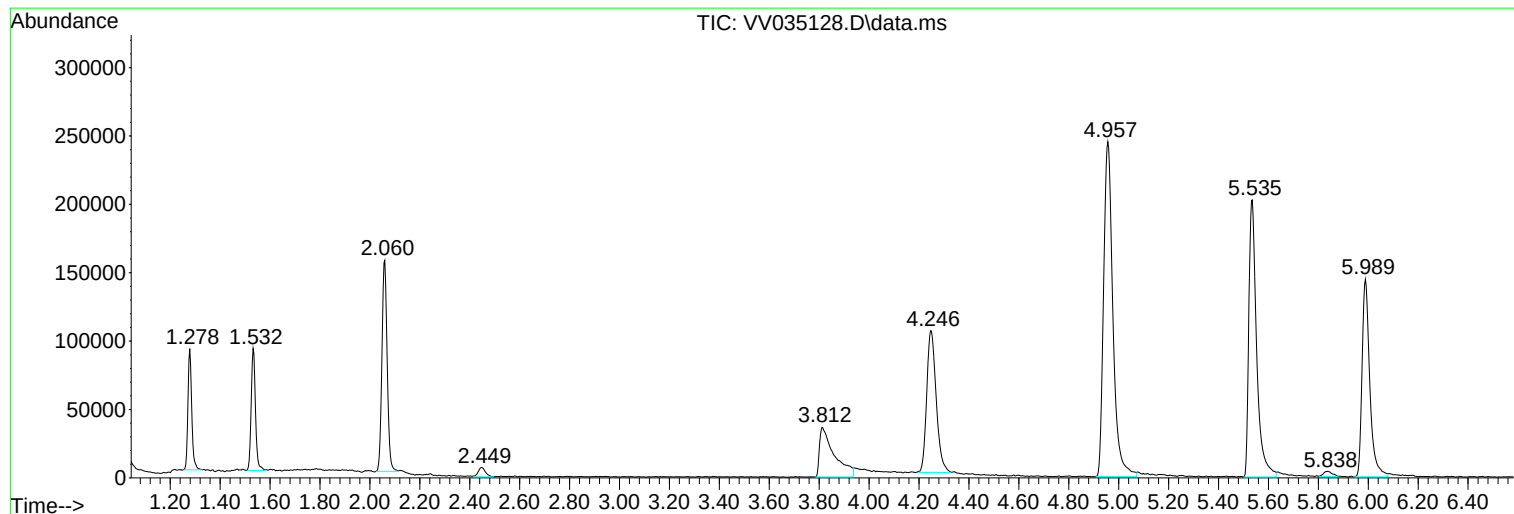

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035128.D
Acq On : 11 Apr 2024 16:54
Operator : SY/MD
Sample : VV0411WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035128.D
Acq On : 11 Apr 2024 16:54
Operator : SY/MD
Sample : VV0411WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc