

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035139.D
 Acq On : 11 Apr 2024 21:18
 Operator : SY/MD
 Sample : P2056-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rBV	82026	86945	10.82%	1.592%
2	1.359	93	99	103	rBV2	11691	15189	1.89%	0.278%
3	1.384	104	107	115	rVB	12436	13774	1.71%	0.252%
4	1.535	145	154	165	rBV	79497	94400	11.74%	1.728%
5	2.060	307	317	332	rBV	147434	216639	26.95%	3.967%
6	2.561	464	473	483	rVB3	5759	11532	1.43%	0.211%
7	3.828	848	867	921	rBV2	145963	803902	100.00%	14.719%
8	4.249	984	998	1029	rVB2	95685	256617	31.92%	4.699%
9	4.957	1204	1218	1252	rBV3	226822	590373	73.44%	10.809%
10	5.535	1385	1398	1427	rBV	172176	375392	46.70%	6.873%
11	5.834	1483	1491	1510	rVB	4933	11099	1.38%	0.203%
12	5.989	1527	1539	1565	rBV	131554	284995	35.45%	5.218%
13	6.918	1817	1828	1855	rBV2	46530	99065	12.32%	1.814%
14	7.243	1918	1929	1954	rBV	233020	430914	53.60%	7.890%
15	7.561	2019	2028	2051	rBV2	27410	58435	7.27%	1.070%
16	7.911	2128	2137	2151	rVB5	9945	19388	2.41%	0.355%
17	8.030	2165	2174	2217	rBV2	260889	635589	79.06%	11.637%
18	8.786	2396	2409	2433	rBV	276738	481231	59.86%	8.811%
19	10.152	2822	2834	2858	rBV	101913	167402	20.82%	3.065%
20	11.185	3145	3155	3176	rBV	257651	421704	52.46%	7.721%
21	11.561	3261	3272	3293	rBV	236485	387080	48.15%	7.087%




Sum of corrected areas: 5461665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035139.D
Acq On : 11 Apr 2024 21:18
Operator : SY/MD
Sample : P2056-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

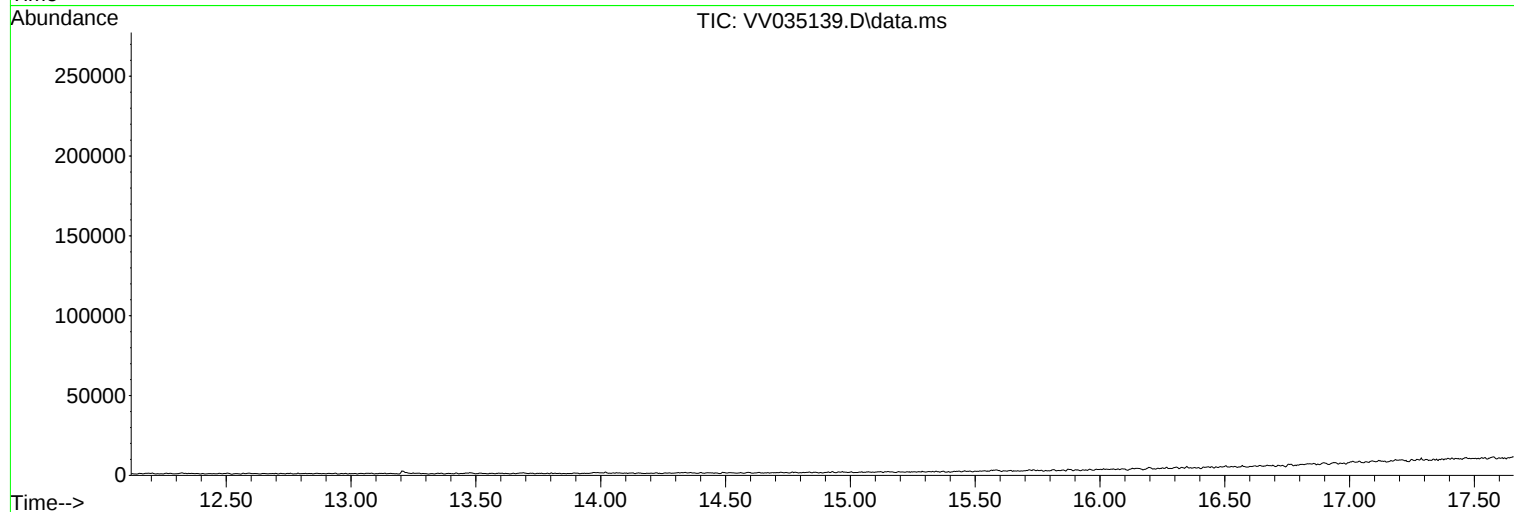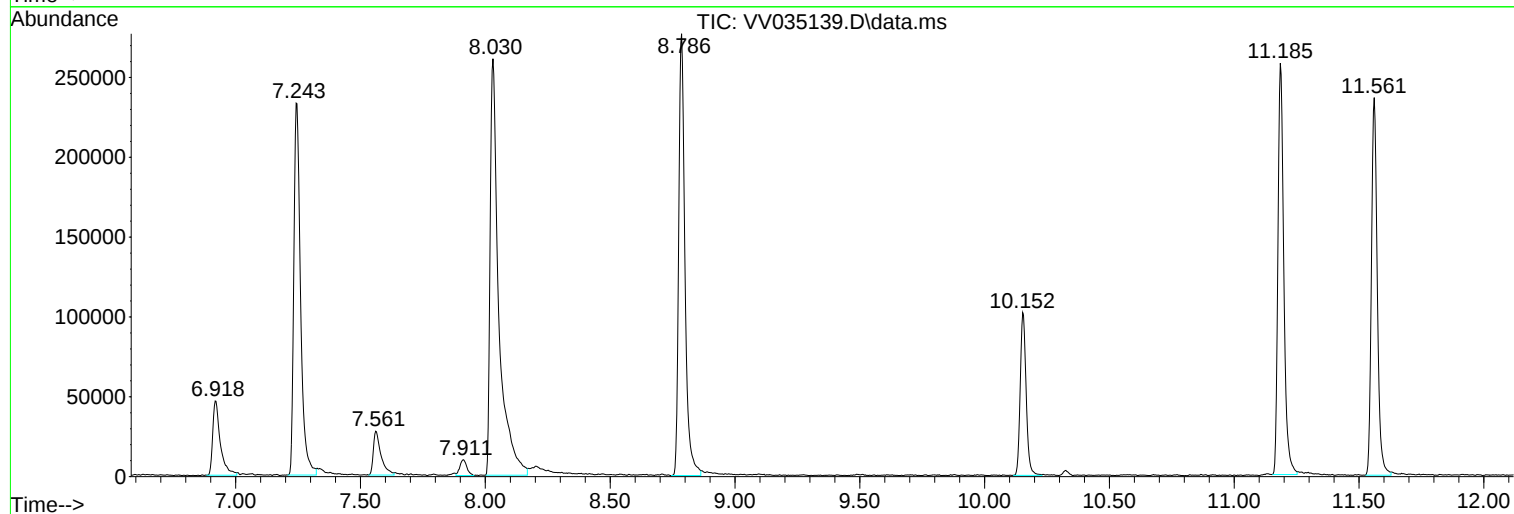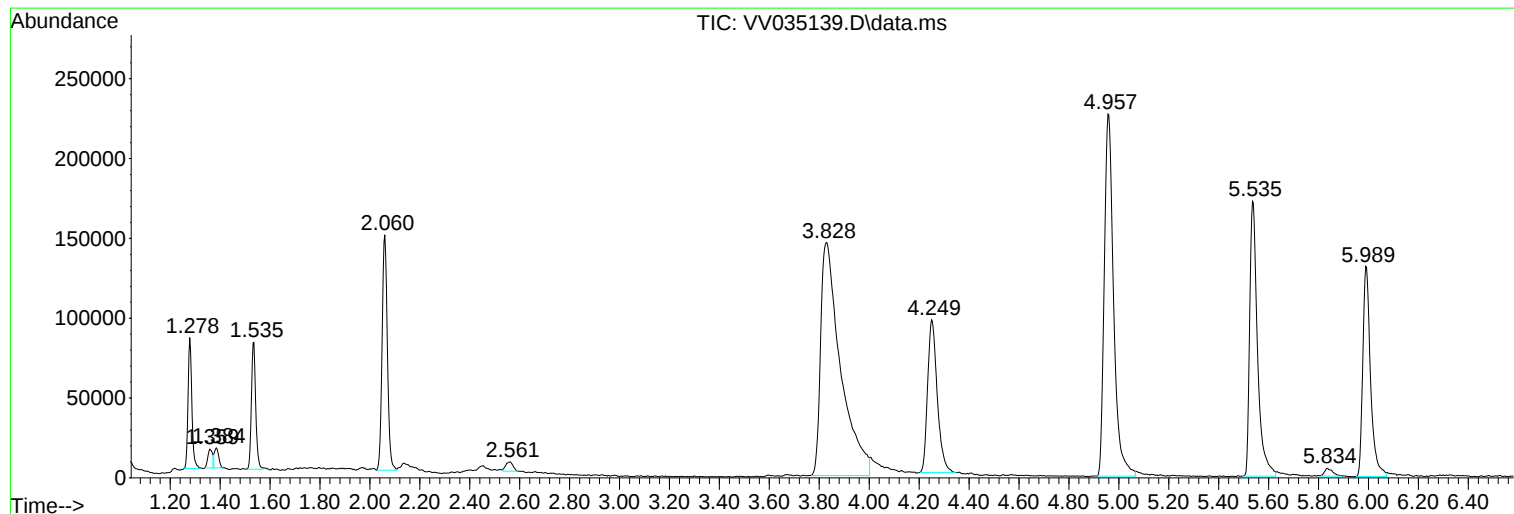

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035139.D
Acq On : 11 Apr 2024 21:18
Operator : SY/MD
Sample : P2056-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035139.D
Acq On : 11 Apr 2024 21:18
Operator : SY/MD
Sample : P2056-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc