

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035145.D
 Acq On : 12 Apr 2024 00:30
 Operator : SY/MD
 Sample : P2057-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BL2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	86	rVB	86585	91650	14.47%	1.753%
2	1.535	146	154	166	rVB	86820	101708	16.06%	1.945%
3	1.973	281	290	299	rBV	10038	15911	2.51%	0.304%
4	2.059	306	317	332	rVB	152588	224045	35.38%	4.285%
5	2.651	484	501	504	rBV4	4810	11579	1.83%	0.221%
6	3.818	848	864	903	rBV3	64153	285702	45.11%	5.464%
7	4.249	980	998	1022	rBV	104969	278047	43.90%	5.318%
8	4.960	1204	1219	1258	rBV2	240898	633321	100.00%	12.113%
9	5.535	1385	1398	1427	rBV	189715	408075	64.43%	7.805%
10	5.989	1527	1539	1564	rBV	144194	308916	48.78%	5.908%
11	6.921	1817	1829	1848	rBV2	47728	100176	15.82%	1.916%
12	7.246	1919	1930	1967	rBV	251249	476942	75.31%	9.122%
13	7.561	2017	2028	2047	rBV2	27793	57834	9.13%	1.106%
14	7.879	2114	2127	2131	rBV4	5154	9247	1.46%	0.177%
15	8.027	2164	2173	2217	rBV	278813	627747	99.12%	12.006%
16	8.786	2398	2409	2436	rBV	304260	526477	83.13%	10.069%
17	10.152	2823	2834	2856	rBV	110014	180104	28.44%	3.445%
18	10.323	2878	2887	2899	rVB2	12346	20793	3.28%	0.398%
19	11.184	3142	3155	3183	rBV	280963	455667	71.95%	8.715%
20	11.561	3260	3272	3296	rBV	256955	414625	65.47%	7.930%




Sum of corrected areas: 5228566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035145.D
Acq On : 12 Apr 2024 00:30
Operator : SY/MD
Sample : P2057-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

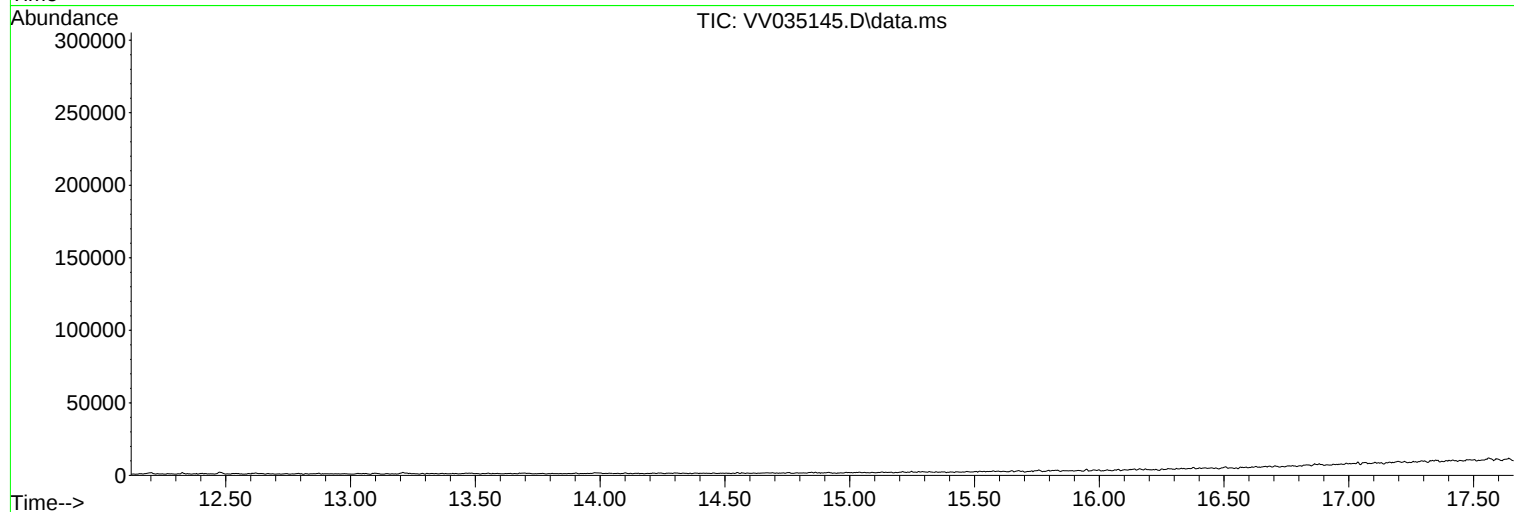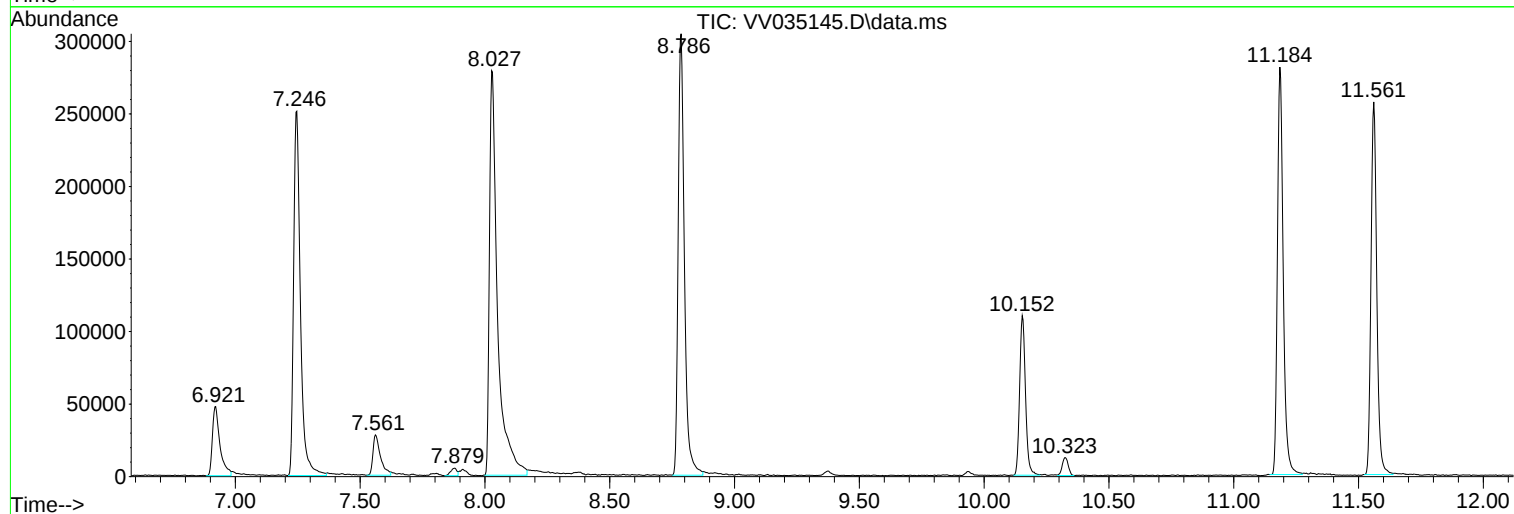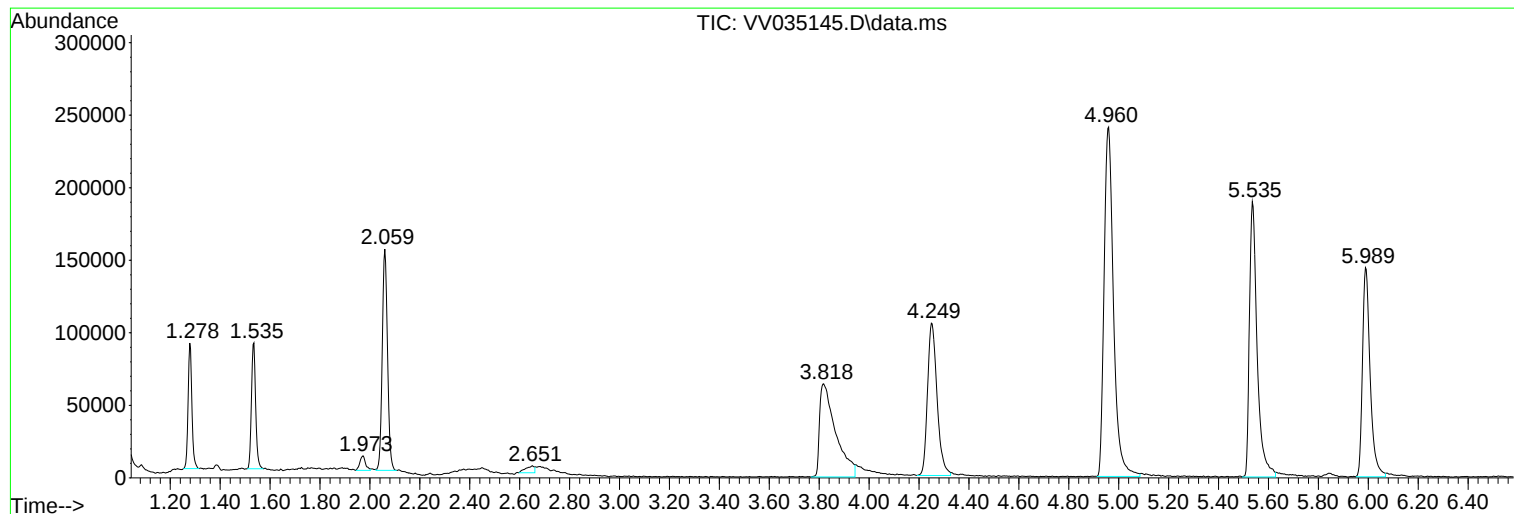

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035145.D
Acq On : 12 Apr 2024 00:30
Operator : SY/MD
Sample : P2057-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035145.D
Acq On : 12 Apr 2024 00:30
Operator : SY/MD
Sample : P2057-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc