

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
 Data File : VV035163.D
 Acq On : 12 Apr 2024 07:41
 Operator : SY/MD
 Sample : P2057-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV035163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	84570	90175	14.48%	1.708%
2	1.388	102	108	117	rVB	15632	18017	2.89%	0.341%
3	1.532	146	153	168	rVB	84994	100754	16.18%	1.908%
4	1.970	281	289	298	rBV2	8969	13880	2.23%	0.263%
5	2.060	306	317	334	rBV	148460	214771	34.48%	4.067%
6	3.815	848	863	917	rBV2	78050	361759	58.08%	6.851%
7	4.249	982	998	1037	rBV2	104069	275086	44.17%	5.209%
8	4.957	1200	1218	1253	rBV2	237786	622810	100.00%	11.794%
9	5.535	1387	1398	1432	rBV	185791	404958	65.02%	7.669%
10	5.989	1527	1539	1567	rBV2	143326	308230	49.49%	5.837%
11	6.918	1819	1828	1848	rBV	45368	94521	15.18%	1.790%
12	7.243	1919	1929	1953	rBV	243519	450000	72.25%	8.522%
13	7.561	2019	2028	2046	rBV2	26002	53906	8.66%	1.021%
14	7.908	2125	2136	2152	rVB	39936	71564	11.49%	1.355%
15	8.027	2164	2173	2211	rBV	283345	621907	99.86%	11.777%
16	8.786	2398	2409	2439	rBV	308301	525710	84.41%	9.956%
17	10.152	2823	2834	2852	rBV	111731	179492	28.82%	3.399%
18	10.326	2879	2888	2897	rVB2	4530	6907	1.11%	0.131%
19	11.185	3143	3155	3180	rBV	286815	456672	73.32%	8.648%
20	11.561	3259	3272	3296	rBV	245237	409409	65.74%	7.753%




Sum of corrected areas: 5280528

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035163.D
Acq On : 12 Apr 2024 07:41
Operator : SY/MD
Sample : P2057-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

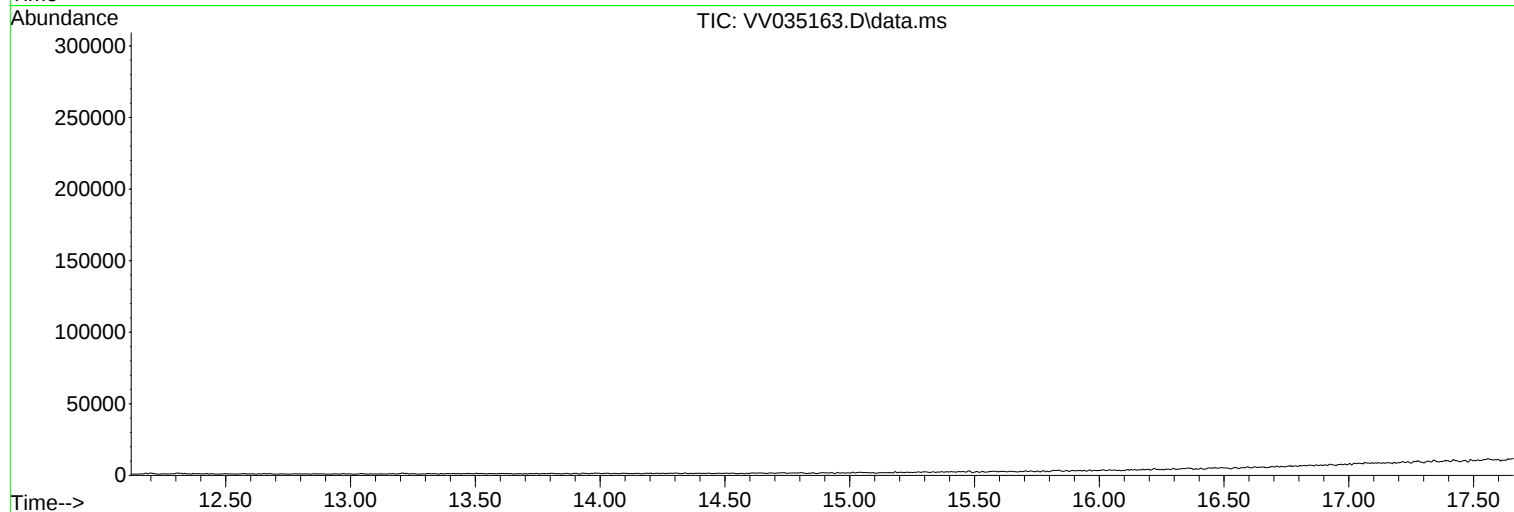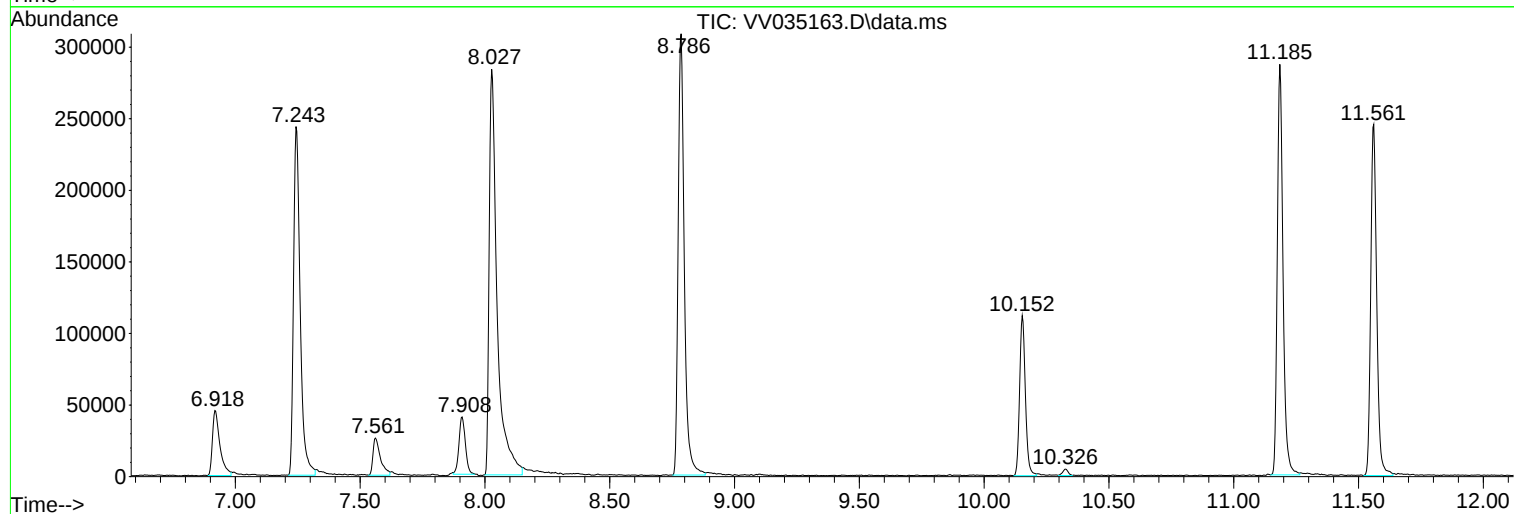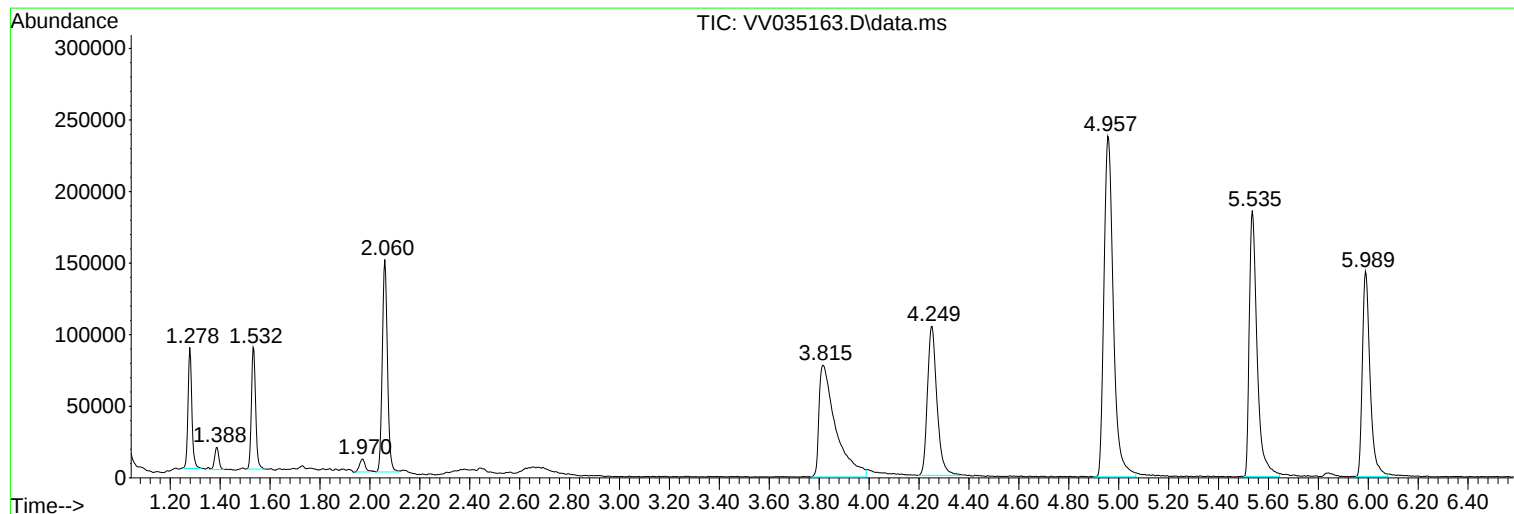

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035163.D
Acq On : 12 Apr 2024 07:41
Operator : SY/MD
Sample : P2057-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035163.D
Acq On : 12 Apr 2024 07:41
Operator : SY/MD
Sample : P2057-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc