


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041124\
Data File : VV035126.D
Acq On : 11 Apr 2024 13:00
Operator : SY/MD
Sample : BFB266
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB266

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Apr 13 03:40:41 2024

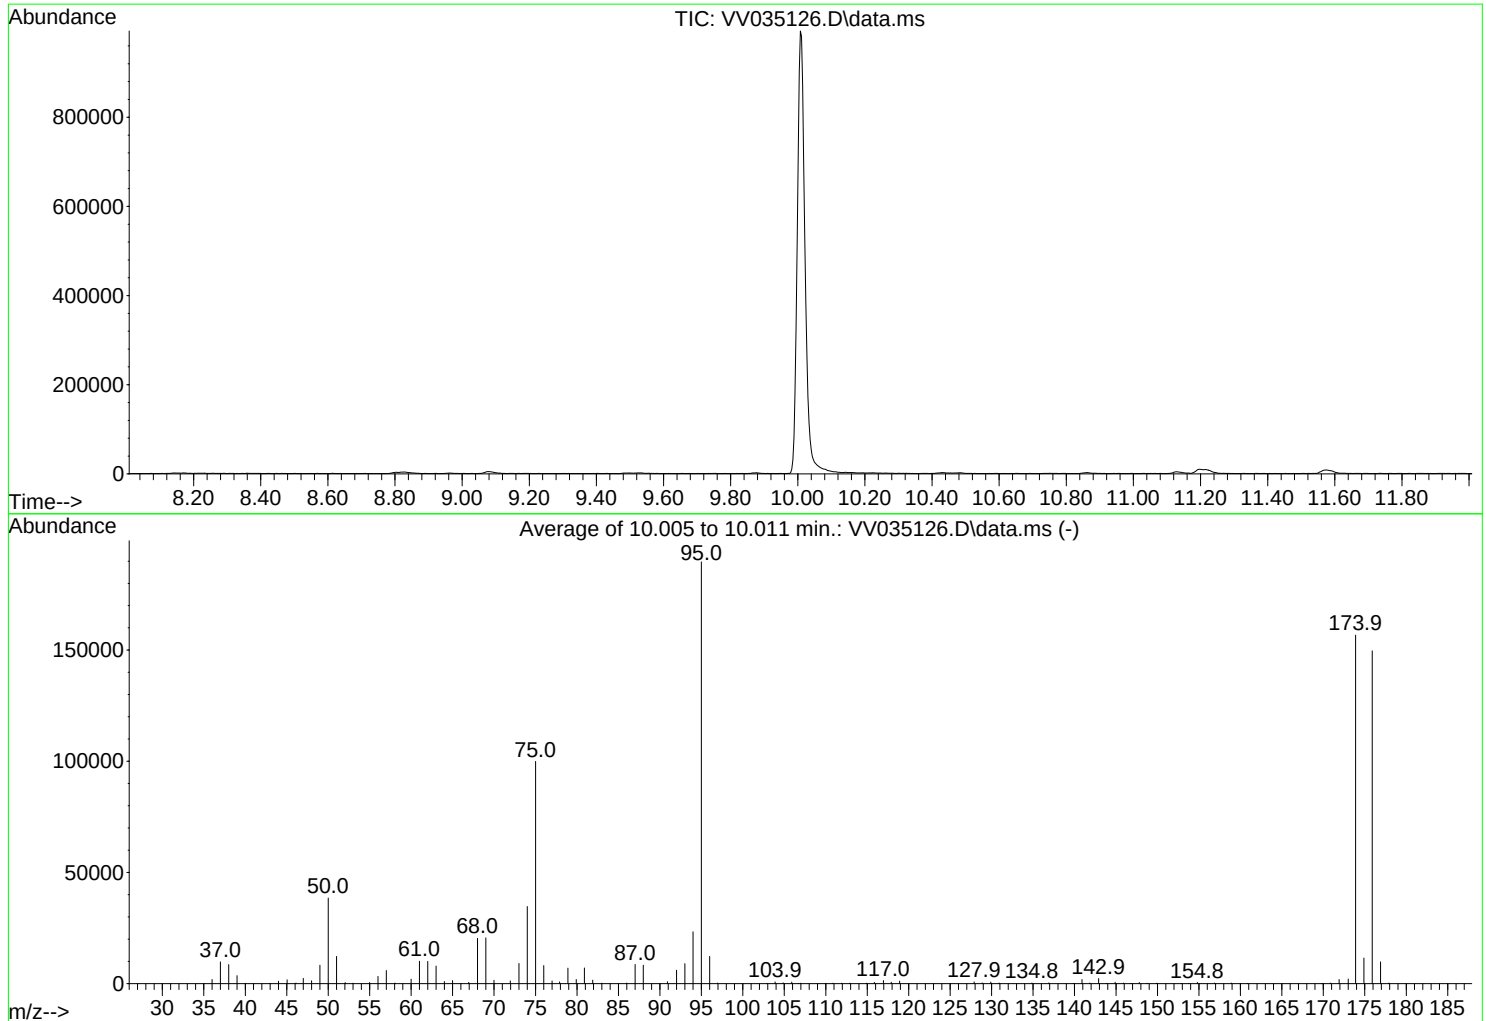

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	38525	PASS
75	95	30	80	52.7	99947	PASS
95	95	100	100	100.0	189696	PASS
96	95	5	9	6.4	12212	PASS
173	174	0.00	2	1.3	2079	PASS
174	95	50	120	82.6	156757	PASS
175	174	5	9	7.3	11486	PASS
176	174	95	105	95.5	149675	PASS
177	176	5	10	6.6	9821	PASS

m/z	Abundance
40.00	238.0
44.00	568.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

m/z	Abundance
36.00	1745.0
37.00	9401.0
38.00	8247.0
39.00	3561.0
40.00	370.0
42.90	110.0
44.00	1585.0
45.10	1726.0
46.20	346.0
47.00	2343.0
48.00	1256.0
49.00	7814.0
50.00	37064.0
51.00	11785.0
52.10	489.0
53.00	253.0
55.00	440.0
56.00	3176.0
57.00	5797.0
58.00	211.0
60.00	1855.0
61.00	9461.0
62.00	9685.0
63.00	7665.0
64.00	922.0
65.00	1368.0
66.00	198.0
67.00	565.0
68.00	19064.0
69.00	19472.0
70.00	1592.0
72.00	1139.0
73.00	8640.0
74.00	33304.0
75.00	94928.0
76.00	7760.0
77.00	1154.0
77.90	681.0
78.90	6748.0
79.90	1828.0
80.90	6824.0
81.90	1484.0
83.00	220.0
86.00	216.0
87.00	8223.0
88.00	8050.0
90.90	783.0
92.00	5472.0
93.00	8670.0
94.00	22480.0
95.00	179968.0
96.00	11744.0
97.00	253.0
102.90	113.0
103.90	780.0
104.80	332.0
105.90	645.0
106.90	186.0
110.00	148.0
110.90	174.0
111.90	165.0
112.90	203.0
114.90	234.0
115.90	527.0
117.00	1296.0
117.90	695.0
118.90	1116.0
127.90	716.0
128.80	350.0
129.90	660.0
130.90	296.0
134.80	311.0
136.90	286.0
139.90	122.0
140.90	1785.0
141.90	282.0
142.90	2187.0
143.80	115.0
144.90	591.0
145.90	332.0
146.80	135.0
147.80	510.0
148.70	181.0
149.90	216.0
152.90	176.0
153.70	101.0
154.80	464.0
156.90	305.0
158.90	293.0
160.80	155.0
170.80	274.0
171.90	1835.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

173.00	2027.0
173.90	143104.0
174.90	10691.0
175.90	137920.0
176.90	9385.0
177.90	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

m/z	Abundance
36.00	1971.0
37.00	10268.0
38.00	8850.0
39.00	3794.0
40.00	425.0
43.00	138.0
44.00	1637.0
45.00	1808.0
46.10	324.0
47.00	2457.0
48.00	1394.0
49.00	8570.0
50.00	39800.0
51.00	12729.0
52.10	580.0
53.00	240.0
55.00	528.0
56.00	3448.0
57.00	6042.0
58.00	278.0
60.00	2092.0
61.00	10404.0
62.00	10372.0
63.00	8137.0
64.00	963.0
65.00	1438.0
66.00	168.0
66.90	602.0
68.00	21176.0
69.00	21296.0
70.00	1561.0
72.00	1229.0
73.00	9323.0
74.00	35880.0
75.00	103752.0
76.00	8376.0
77.00	1277.0
77.90	798.0
78.90	7244.0
79.90	1926.0
80.90	7305.0
81.90	1653.0
83.00	228.0
86.00	252.0
87.00	8905.0
88.00	8630.0
90.90	899.0
92.00	6312.0
93.00	9361.0
94.00	24144.0
95.00	196736.0
96.00	12519.0
96.90	279.0
102.90	121.0
103.90	852.0
104.90	387.0
105.90	696.0
107.00	191.0
110.00	139.0
110.80	237.0
111.90	229.0
112.90	214.0
114.90	249.0
115.80	603.0
116.90	1416.0
117.90	691.0
118.90	1166.0
127.90	836.0
128.90	331.0
129.90	783.0
130.90	333.0
134.80	328.0
136.90	375.0
139.80	146.0
140.90	1970.0
141.90	258.0
142.90	2434.0
143.90	138.0
144.90	639.0
145.90	308.0
146.80	139.0
147.80	485.0
148.80	199.0
149.90	203.0
152.80	164.0
153.70	106.0
154.80	574.0
156.90	329.0
158.90	313.0
160.90	174.0
170.90	283.0
171.90	1964.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

173.00	2153.0
173.90	162304.0
174.90	11885.0
175.90	155008.0
176.90	10196.0
177.90	336.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

m/z	Abundance
36.00	1934.0
37.00	9757.0
38.00	8559.0
39.00	3515.0
40.00	423.0
43.00	158.0
44.00	1645.0
45.00	1717.0
46.00	278.0
47.00	2253.0
48.00	1314.0
49.00	8428.0
50.00	38712.0
51.00	12252.0
52.00	511.0
53.00	231.0
55.00	588.0
56.00	3198.0
57.00	5847.0
58.10	326.0
60.00	2041.0
61.00	10416.0
62.00	9993.0
63.00	7959.0
64.00	869.0
65.00	1415.0
66.00	171.0
67.00	589.0
68.00	20936.0
69.00	21000.0
70.00	1408.0
71.90	1247.0
73.00	9226.0
74.00	34960.0
75.00	101160.0
76.00	8237.0
77.00	1250.0
77.90	939.0
78.90	6896.0
79.90	1928.0
80.90	7019.0
81.90	1666.0
83.00	204.0
86.00	299.0
87.00	8743.0
88.00	8255.0
90.90	840.0
92.00	6367.0
93.00	9079.0
94.00	23288.0
95.00	192384.0
96.00	12373.0
97.00	305.0
102.90	126.0
103.90	859.0
104.90	379.0
105.90	784.0
106.70	177.0
107.00	182.0
109.90	120.0
110.80	251.0
111.90	235.0
112.90	207.0
114.90	246.0
115.80	651.0
116.90	1349.0
117.90	655.0
118.90	1126.0
127.90	819.0
128.90	331.0
129.90	797.0
130.90	285.0
134.90	304.0
136.90	406.0
139.90	141.0
140.90	1918.0
141.80	227.0
142.90	2316.0
143.90	142.0
144.90	619.0
145.90	238.0
146.80	124.0
147.80	428.0
148.80	204.0
149.90	199.0
152.80	135.0
153.80	125.0
154.80	602.0
156.90	322.0
158.90	261.0
160.80	199.0
169.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

170.90	234.0
171.90	1900.0
173.00	2056.0
173.90	164864.0
174.90	11883.0
175.90	156096.0
176.90	9882.0
177.90	384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266