

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041219\
Quantitation Report (QT Reviewed)


Data File : VV010289.D
Acq On : 12 Apr 2019 15:57
Operator : SY/MD
Sample : K2304-05RE
Misc : 4.85G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF890RE

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:31:26 AM

Quant Time: Apr 13 05:29:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:47:32 2019
Response via : Initial Calibration

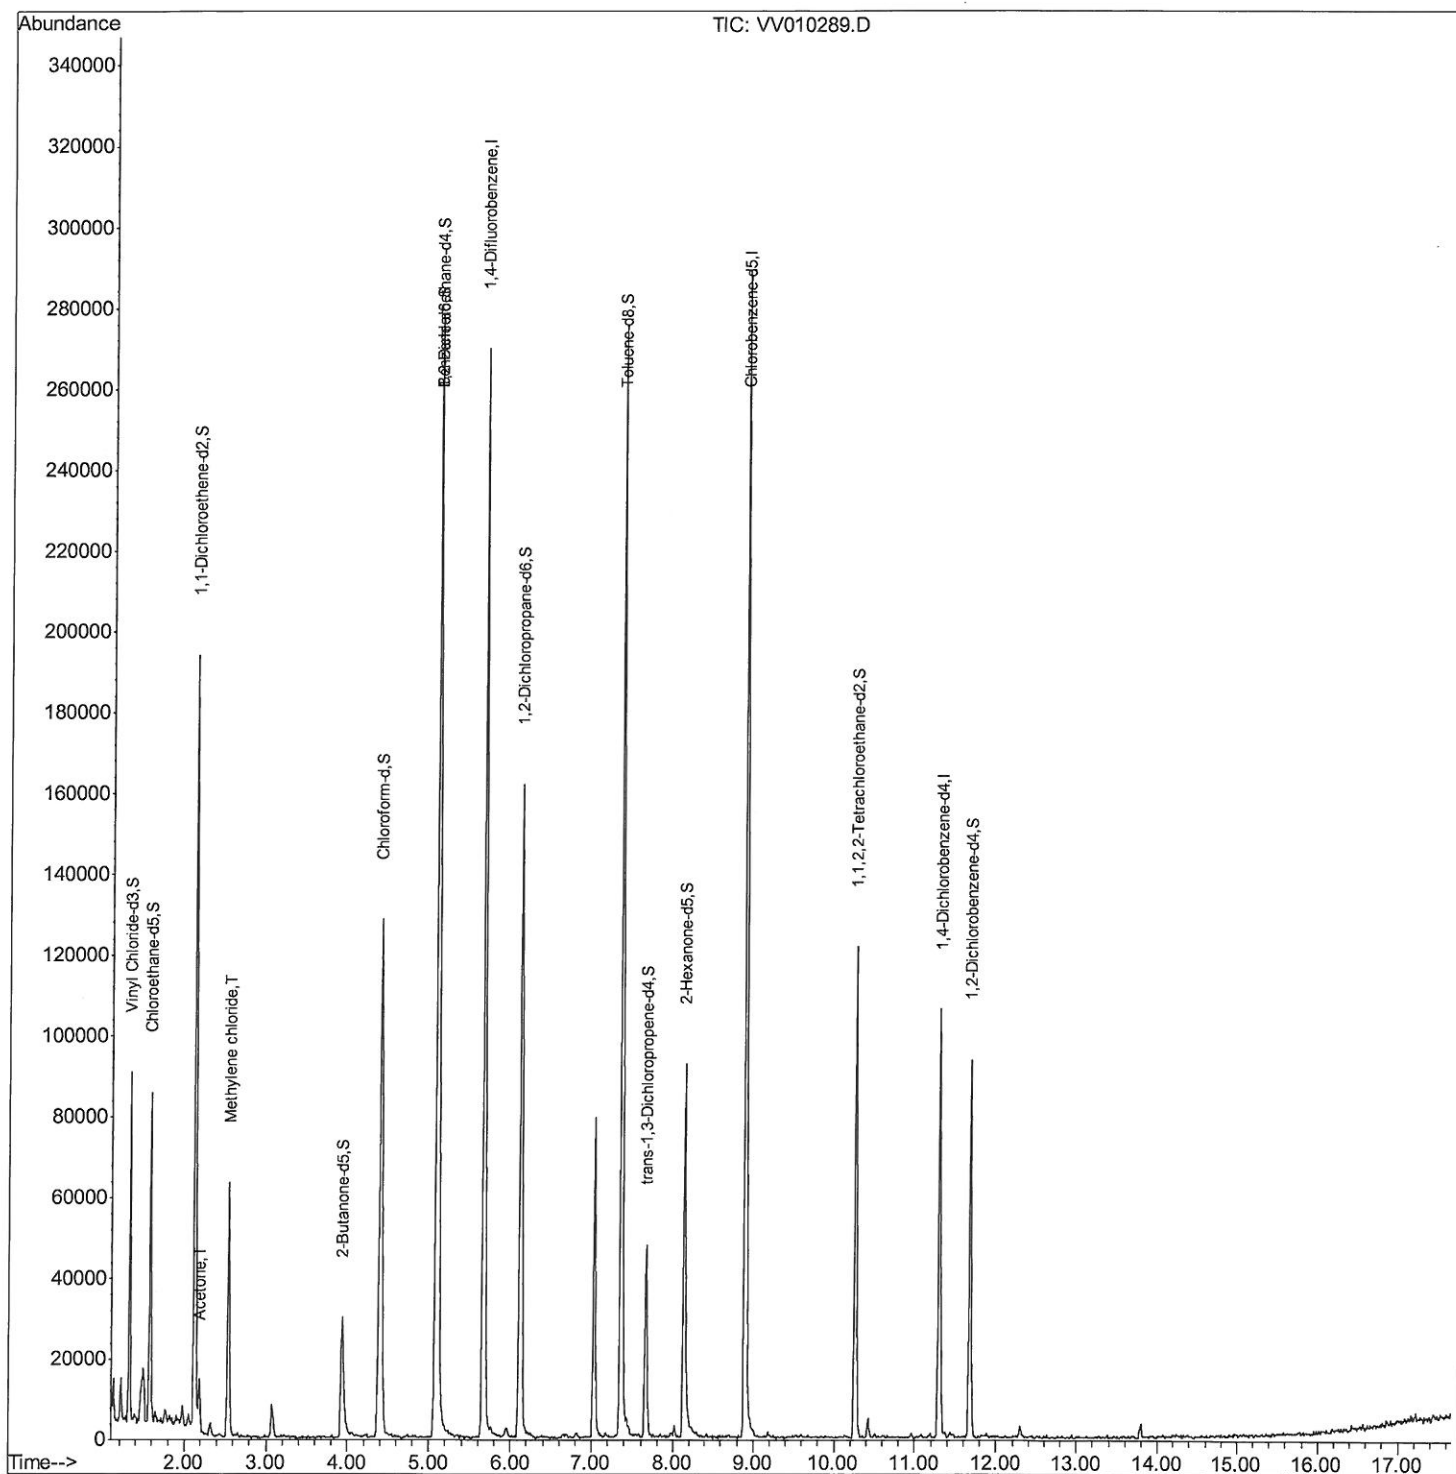

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041219\
Quantitation Report (Qedit)




Data File : VV010289.D
Acq On : 12 Apr 2019 15:57
Operator : SY/MD
Sample : K2304-05RE
Misc : 4.85G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF890RE

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:31:26 AM

Quant Time: Apr 13 04:52:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:47:32 2019
Response via : Initial Calibration

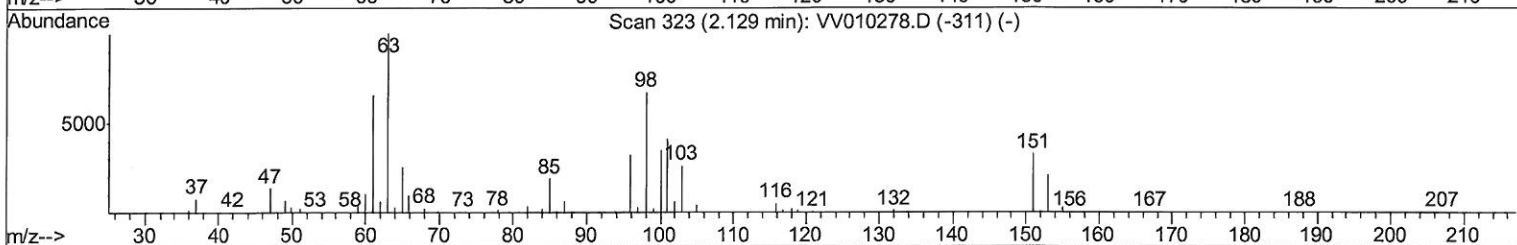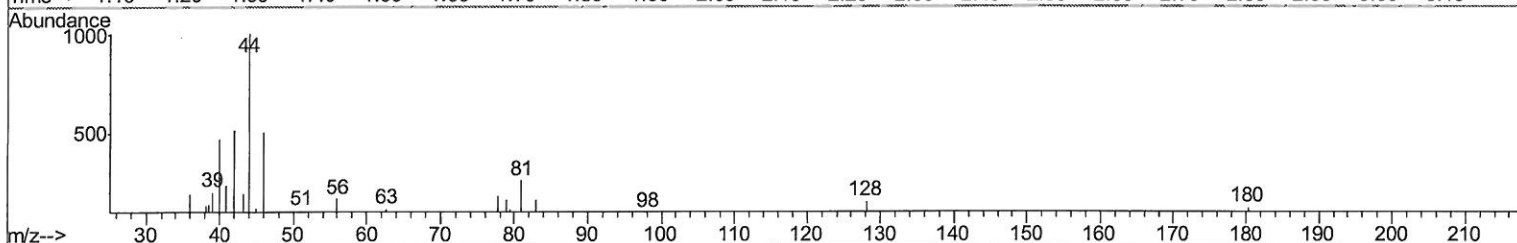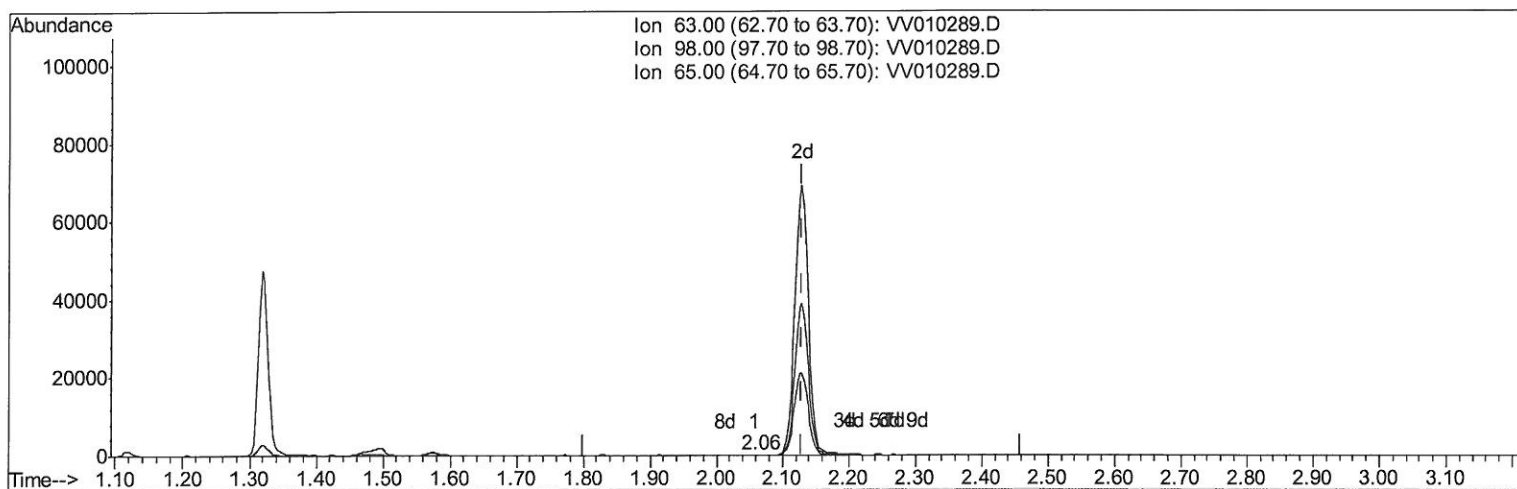

TIC: VV010289.D

(10) 1,1-Dichloroethene-d2 (S)

2.058min (-0.071) 0.01ug/L

response 64

Ion	Exp%	Act%
63.00	100	100
98.00	71.30	64.06
65.00	23.70	29.69
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041219\
Quantitation Report (Qedit)




Data File : VV010289.D
Acq On : 12 Apr 2019 15:57
Operator : SY/MD
Sample : K2304-05RE
Misc : 4.85G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF890RE

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:31:26 AM

Quant Time: Apr 13 04:52:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:47:32 2019
Response via : Initial Calibration

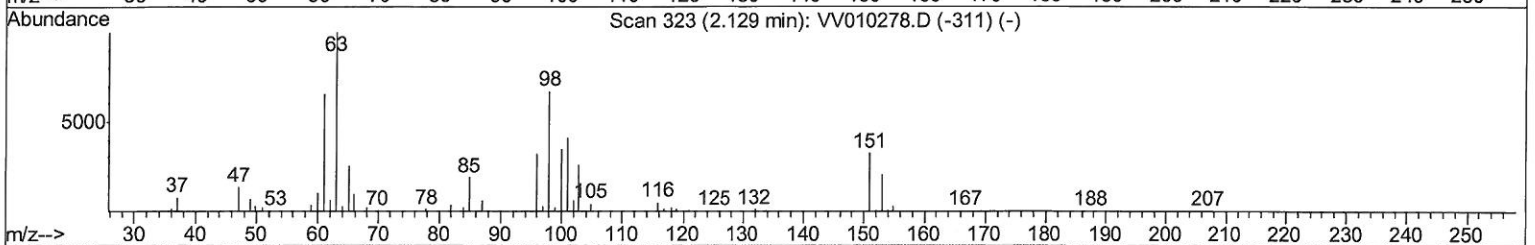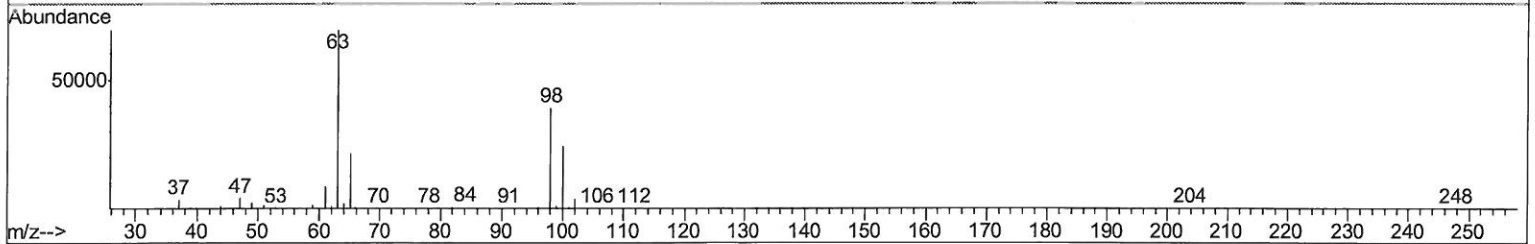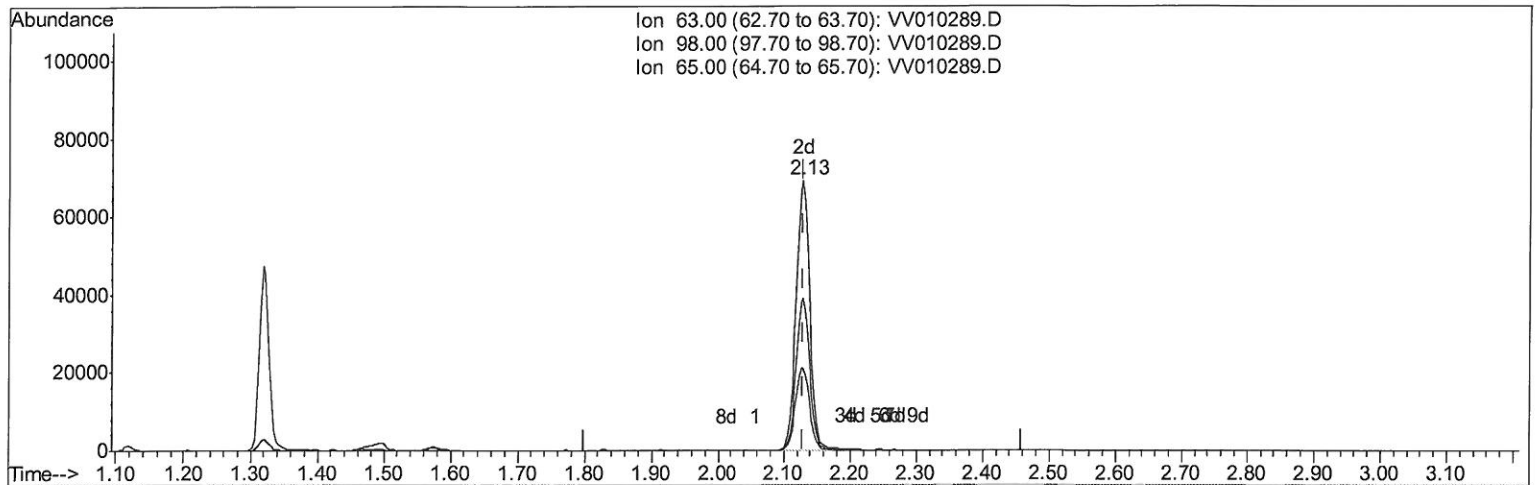

TIC: VV010289.D

(10) 1,1-Dichloroethene-d2 (S)

2.129min (-0.000) 14.27ug/L m

response 97676

Ion	Exp%	Act%
63.00	100	100
98.00	71.30	0.04#
65.00	23.70	0.02#
0.00	0.00	0.00

7MD
4/16/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041219\
Quantitation Report (QT Reviewed)

Data File : VV010289.D
Acq On : 12 Apr 2019 15:57
Operator : SY/MD
Sample : K2304-05RE
Misc : 4.85G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF890RE

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:31:26 AM

Quant Time: Apr 13 05:29:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:47:32 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	233586	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	164148	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	32699	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46428	17.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.08%
7) Chloroethane-d5	1.58	69	51988	22.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.00%
10) 1,1-Dichloroethene-d2	2.13	63	97676m	14.27	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.08%
20) 2-Butanone-d5	3.93	46	46675	68.59	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	137.18%#
24) Chloroform-d	4.40	84	127094	23.83	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.32%
26) 1,2-Dichloroethane-d4	5.08	65	78727	25.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.64%
29) Benzene-d6	5.10	84	232815	29.41	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	117.64%
33) 1,2-Dichloropropane-d6	6.12	67	72901	30.97	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	123.88%#
37) Toluene-d8	7.36	98	184239	23.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.48%
38) trans-1,3-Dichloropropene-	7.66	79	25324	25.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	103.20%
39) 2-Hexanone-d5	8.13	63	29644	72.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	145.80%#
48) 1,1,2,2-Tetrachloroethane-	10.26	84	54203	25.65	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.60%
61) 1,2-Dichlorobenzene-d4	11.68	152	26877	22.26	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.04%

7MD
4/16/19

Target Compounds					Qvalue
13) Acetone	2.19	43	11437	15.731 ug/L	99
16) Methylene chloride	2.54	84	25174	5.503 ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed