




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030512.D
Acq On : 12 Apr 2023 12:53
Operator : SY/MD
Sample : VV0412WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:47:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 13 02:44:31 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/14/2023
Supervised By :Mahesh Dadoda 04/14/2023

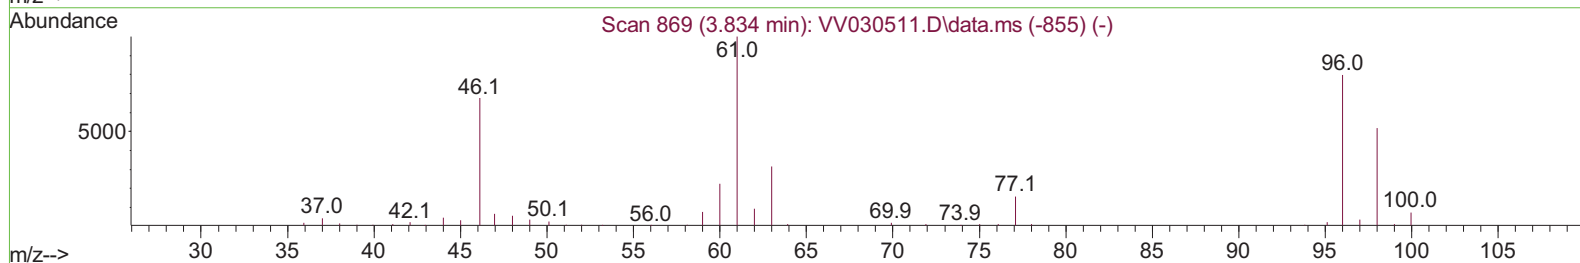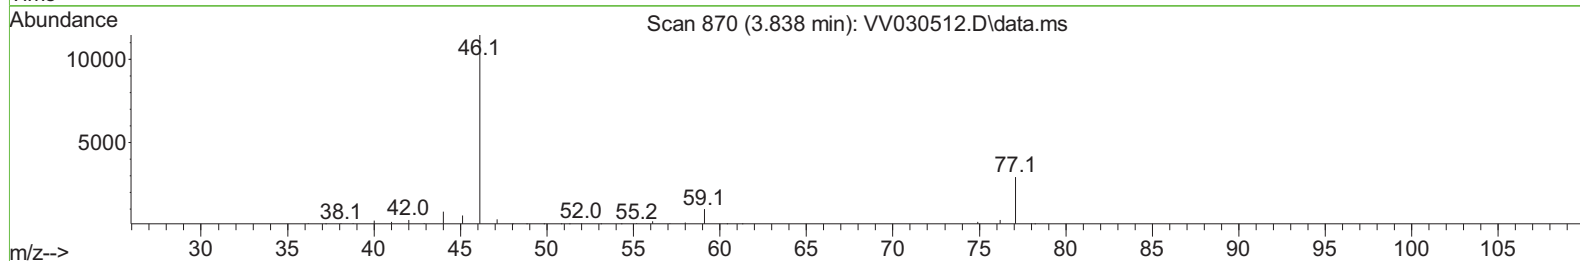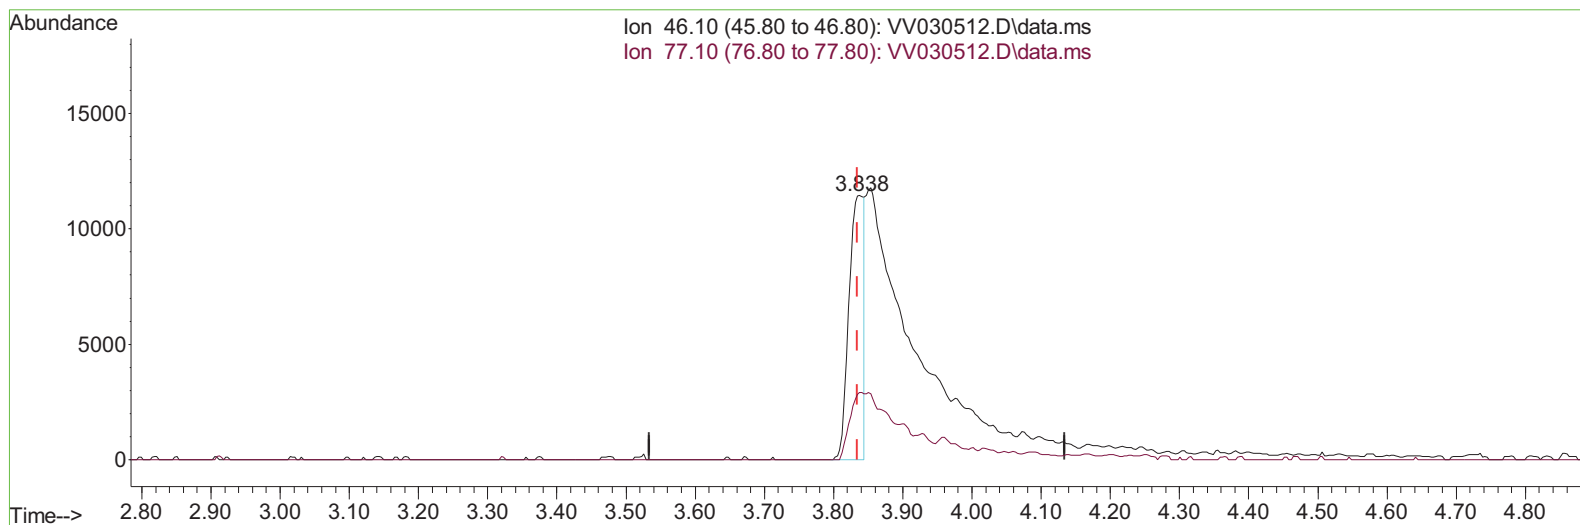

TIC: VV030512.D\data.ms

(20) 2-Butanone-d5 (S)

3.838min (+ 0.003) 9.28 ug/L

response 17505

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	11.10	24.15#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
 Data File : VV030512.D
 Acq On : 12 Apr 2023 12:53
 Operator : SY/MD
 Sample : VV0412WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK327

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:47:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 13 02:44:31 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/14/2023
 Supervised By :Mahesh Dadoda 04/14/2023

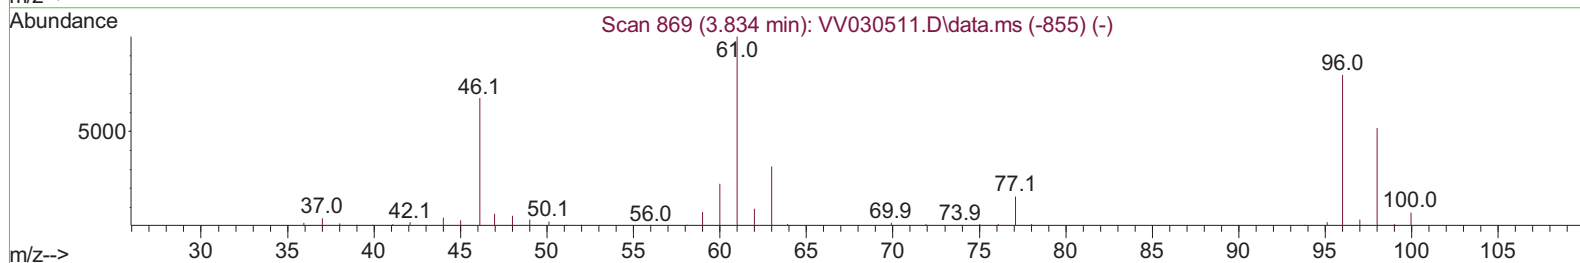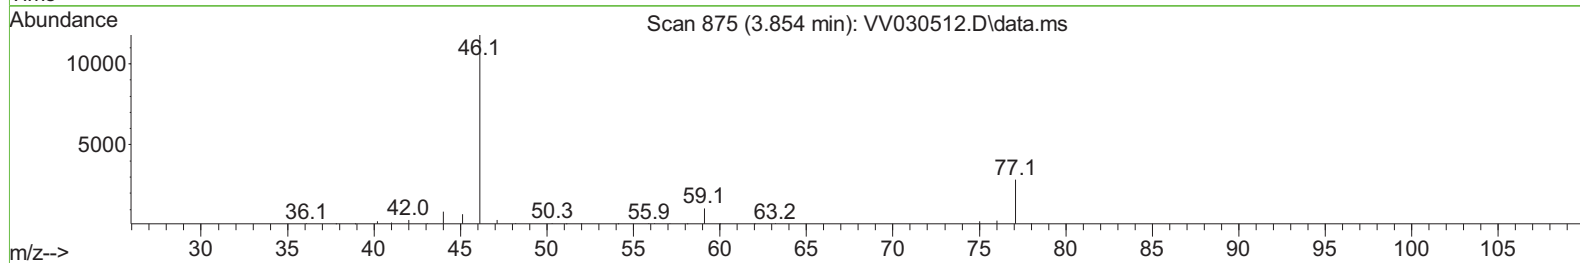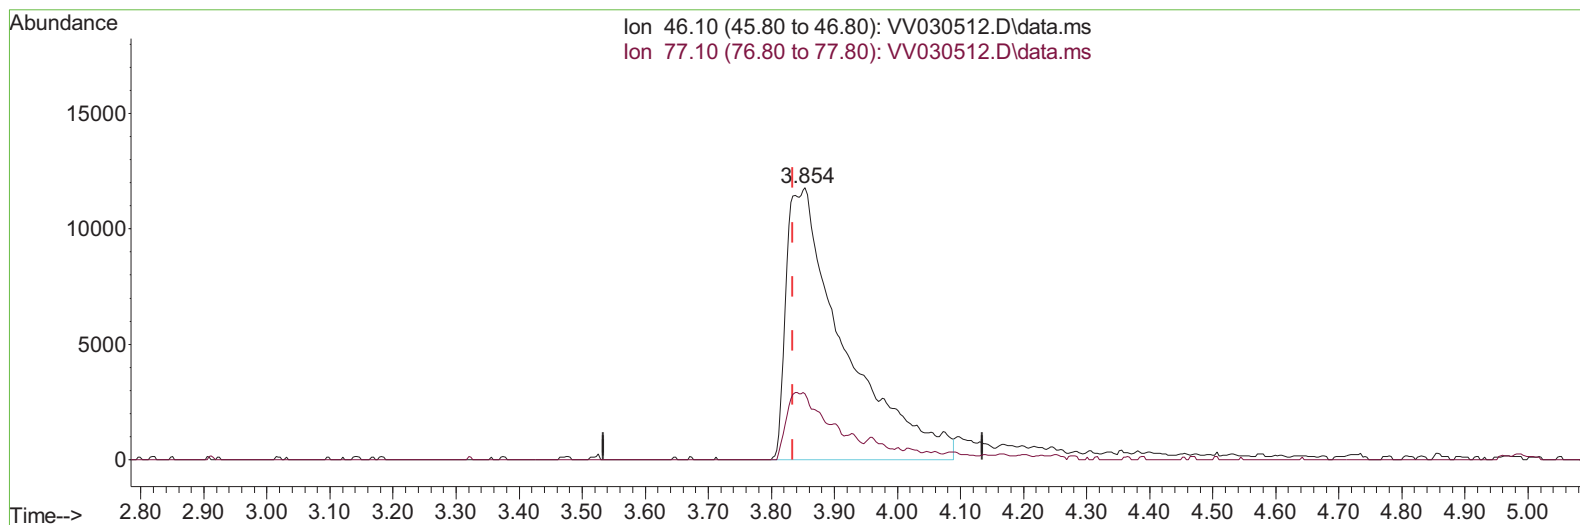

TIC: VV030512.D\data.ms

(20) 2-Butanone-d5 (S)

3.854min (+ 0.019) 39.78 ug/L m

response 75024

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	11.10	5.64#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
 Data File : VV030512.D
 Acq On : 12 Apr 2023 12:53
 Operator : SY/MD
 Sample : VV0412WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK327

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/14/2023
 Supervised By :Mahesh Dadoda 04/14/2023

Quant Time: Apr 13 02:47:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 13 02:44:31 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		110172	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.796	117		111038	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		52963	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		30861	4.229	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.600%	
7) Chloroethane-d5	1.535	69		30326	4.283	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%	
11) 1,1-Dichloroethene-d2	2.063	63		57610	3.327	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.600%	
20) 2-Butanone-d5	3.854	46		75024m	39.780	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.560%	
24) Chloroform-d	4.262	84		79642	4.510	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.200%	
26) 1,2-Dichloroethane-d4	4.953	65		39917	4.791	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%	
32) Benzene-d6	4.973	84		141477	4.522	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	5.998	67		44476	4.540	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.800%	
41) Toluene-d8	7.252	98		127410	4.434	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.600%	
43) trans-1,3-Dichloroprop...	7.561	79		15208	4.123	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%	
46) 2-Hexanone-d5	8.040	63		55852	37.685	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.380%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		31190	4.040	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.800%	
66) 1,2-Dichlorobenzene-d4	11.570	152		47876	5.058	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%	
Target Compounds							
16) Methylene chloride	2.452	84		3572	0.328	ug/L	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030512.D
Acq On : 12 Apr 2023 12:53
Operator : SY/MD
Sample : VV0412WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:47:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 13 02:44:31 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/14/2023
Supervised By :Mahesh Dadoda 04/14/2023

