

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
 Data File : VV030514.D
 Acq On : 12 Apr 2023 13:42
 Operator : SY/MD
 Sample : 02254-08DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	67	75	87	rBV	43801	50059	9.85%	1.218%
2	1.536	146	154	173	rBV	44595	55971	11.02%	1.361%
3	2.073	308	321	336	rBV4	273305	451675	88.91%	10.986%
4	2.452	435	439	449	rVB5	4845	6615	1.30%	0.161%
5	3.121	629	647	665	rBV2	98334	208914	41.12%	5.082%
6	3.847	857	873	894	rBV	22402	94184	18.54%	2.291%
7	4.265	981	1003	1028	rBV	69479	183307	36.08%	4.459%
8	4.523	1065	1083	1106	rBV	196996	508021	100.00%	12.357%
9	4.970	1205	1222	1242	rBV2	152540	381967	75.19%	9.291%
10	5.545	1387	1401	1418	rBV	120821	254970	50.19%	6.202%
11	6.002	1530	1543	1567	rBV2	90473	192689	37.93%	4.687%
12	6.924	1818	1830	1848	rBV	37402	75175	14.80%	1.829%
13	7.252	1918	1932	1947	rBV	170168	306923	60.42%	7.465%
14	7.564	2018	2029	2041	rBV2	23326	42824	8.43%	1.042%
15	8.040	2167	2177	2216	rBV	136409	309447	60.91%	7.527%
16	8.793	2401	2411	2433	rBV	184189	318977	62.79%	7.759%
17	10.162	2824	2837	2854	rBV	65221	107861	21.23%	2.624%
18	11.194	3146	3158	3175	rBV	179192	293011	57.68%	7.127%
19	11.571	3264	3275	3293	rBV	164809	268630	52.88%	6.534%




Sum of corrected areas: 4111220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030514.D
Acq On : 12 Apr 2023 13:42
Operator : SY/MD
Sample : 02254-08DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

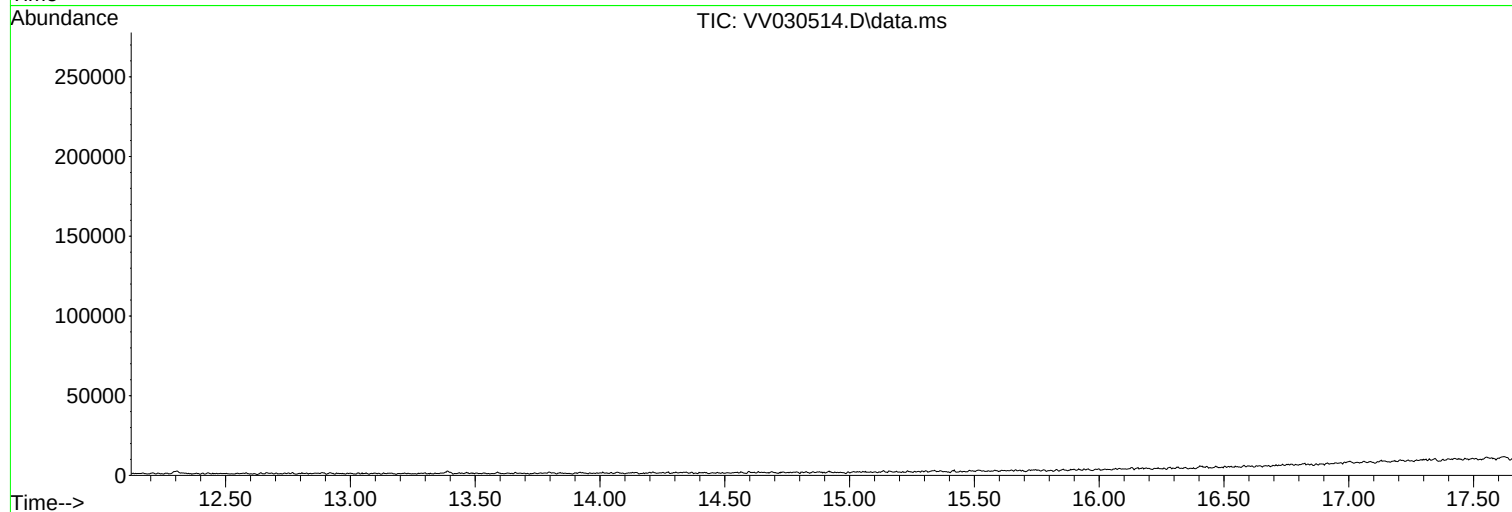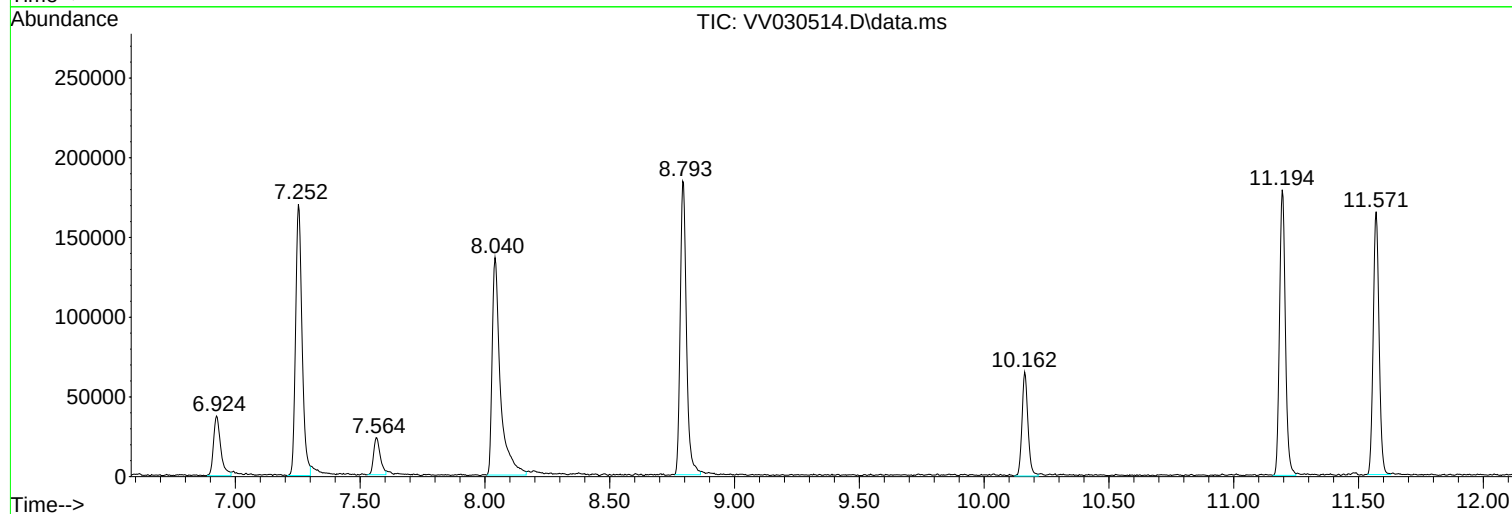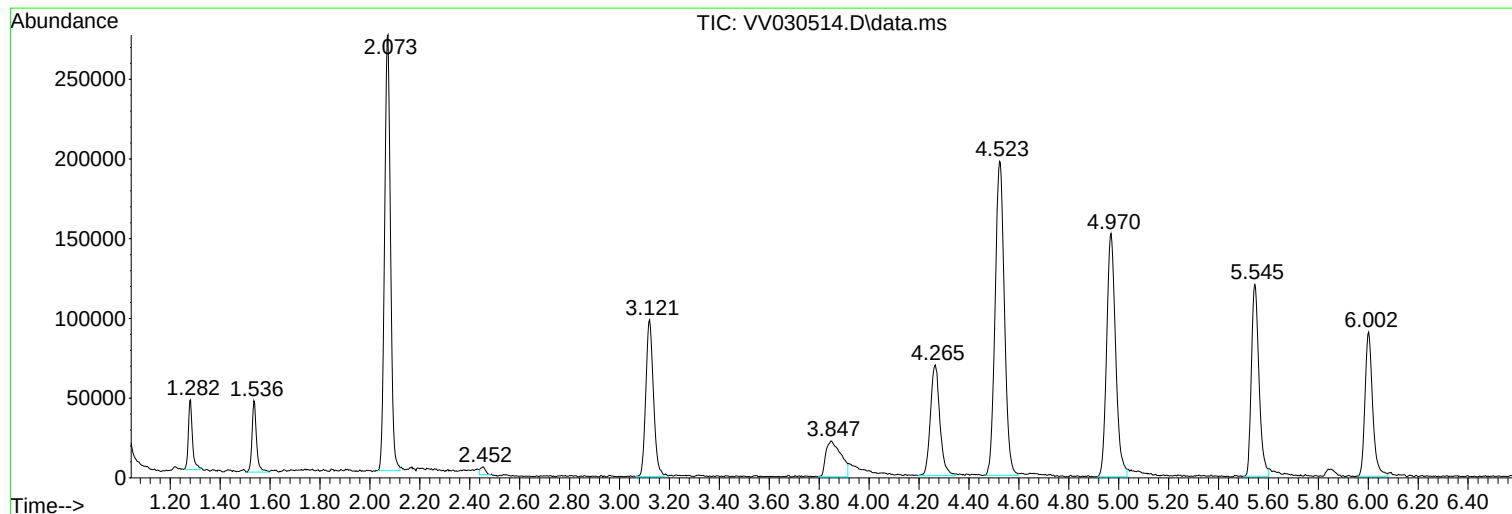

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030514.D
Acq On : 12 Apr 2023 13:42
Operator : SY/MD
Sample : 02254-08DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030514.D
Acq On : 12 Apr 2023 13:42
Operator : SY/MD
Sample : 02254-08DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------