

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
 Data File : VV030523.D
 Acq On : 12 Apr 2023 17:21
 Operator : SY/MD
 Sample : 02250-05DL 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHD6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	68958	77178	17.73%	1.745%
2	1.536	147	154	171	rVB	61010	72809	16.72%	1.646%
3	1.915	267	272	281	rVB	6104	5731	1.32%	0.130%
4	2.069	307	320	336	rBV3	247771	428522	98.42%	9.687%
5	2.458	429	441	454	rVB2	4938	9461	2.17%	0.214%
6	3.124	630	648	664	rBV	28295	62280	14.30%	1.408%
7	3.828	854	867	899	rBV3	45130	183308	42.10%	4.144%
8	4.262	985	1002	1024	rBV	76496	198015	45.48%	4.476%
9	4.526	1071	1084	1101	rVB3	9718	24938	5.73%	0.564%
10	4.969	1204	1222	1243	rBV3	170538	435394	100.00%	9.843%
11	5.545	1387	1401	1422	rBV	128849	274110	62.96%	6.197%
12	5.844	1481	1494	1510	rBV2	188518	380581	87.41%	8.604%
13	6.002	1530	1543	1560	rBV	100775	204711	47.02%	4.628%
14	6.924	1818	1830	1850	rBV2	46183	90353	20.75%	2.043%
15	7.252	1918	1932	1961	rBV	192749	351916	80.83%	7.956%
16	7.564	2019	2029	2053	rBV3	29674	59578	13.68%	1.347%
17	7.915	2123	2138	2151	rBV2	53203	94987	21.82%	2.147%
18	8.037	2166	2176	2204	rBV	188882	391233	89.86%	8.844%
19	8.796	2399	2412	2432	rBV	198336	338988	77.86%	7.663%
20	10.162	2826	2837	2852	rBV	75268	120836	27.75%	2.732%
21	11.194	3147	3158	3176	rBV	199879	314800	72.30%	7.117%
22	11.570	3264	3275	3294	rVB	189192	303780	69.77%	6.867%




Sum of corrected areas: 4423509

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030523.D
Acq On : 12 Apr 2023 17:21
Operator : SY/MD
Sample : 02250-05DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

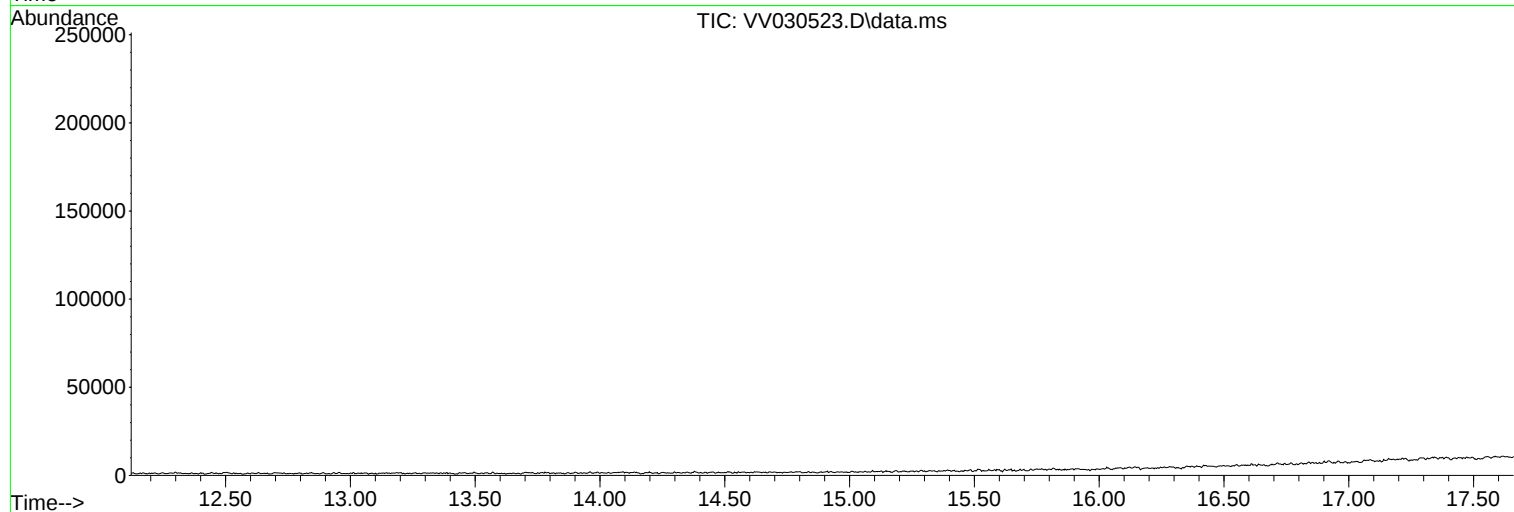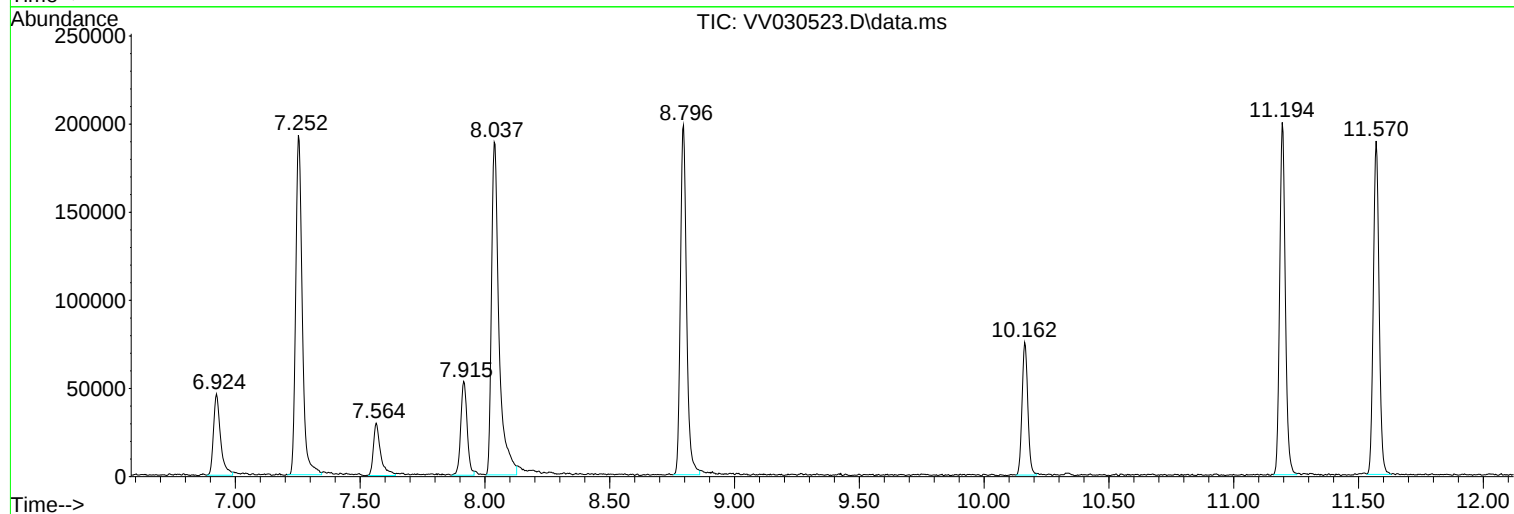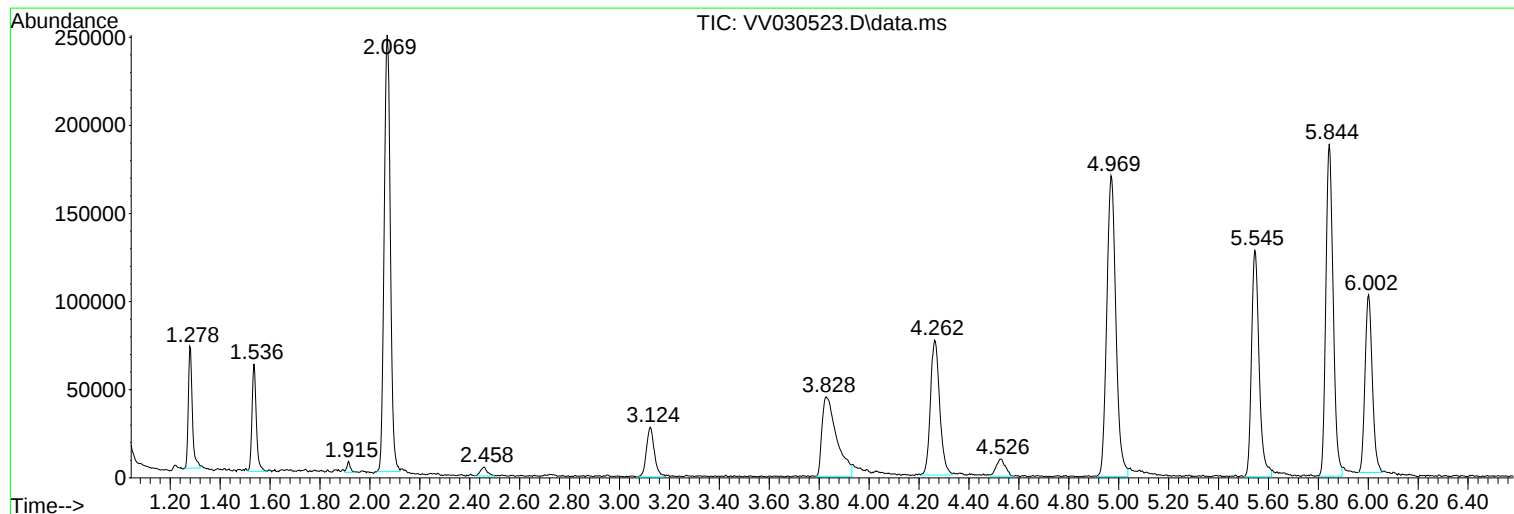

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030523.D
Acq On : 12 Apr 2023 17:21
Operator : SY/MD
Sample : 02250-05DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030523.D
Acq On : 12 Apr 2023 17:21
Operator : SY/MD
Sample : 02250-05DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------