

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
 Data File : VV030526.D
 Acq On : 12 Apr 2023 18:36
 Operator : SY/MD
 Sample : 02275-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rBV	64974	72612	17.22%	1.962%
2	1.536	147	154	169	rBV	55531	68912	16.34%	1.862%
3	2.063	306	318	330	rBV	120020	175905	41.72%	4.754%
4	2.243	364	374	385	rBV2	7309	11915	2.83%	0.322%
5	3.812	848	862	894	rBV2	43404	149486	35.45%	4.040%
6	4.265	984	1003	1024	rBV2	77747	203392	48.24%	5.497%
7	4.966	1205	1221	1247	rBV2	163147	421661	100.00%	11.396%
8	5.545	1388	1401	1426	rBV	130104	275787	65.40%	7.454%
9	5.847	1481	1495	1509	rBV4	13035	28203	6.69%	0.762%
10	5.998	1528	1542	1561	rBV	100253	210040	49.81%	5.677%
11	6.921	1819	1829	1843	rBV2	43272	82688	19.61%	2.235%
12	7.252	1920	1932	1947	rBV	181583	326000	77.31%	8.811%
13	7.326	1947	1955	1969	rVB	20178	41168	9.76%	1.113%
14	7.564	2019	2029	2040	rBV2	29214	53914	12.79%	1.457%
15	7.915	2125	2138	2153	rBV2	37549	64151	15.21%	1.734%
16	8.037	2164	2176	2205	rBV	187660	378224	89.70%	10.222%
17	8.792	2399	2411	2428	rBV	201888	345545	81.95%	9.339%
18	9.506	2622	2633	2645	rBV	4248	9234	2.19%	0.250%
19	10.162	2825	2837	2852	rBV	73756	117620	27.89%	3.179%
20	10.336	2883	2891	2902	rVB4	5473	9089	2.16%	0.246%
21	11.101	3121	3129	3140	rVB9	2840	4886	1.16%	0.132%
22	11.194	3147	3158	3178	rBV	206286	322333	76.44%	8.712%
23	11.570	3264	3275	3290	rBV	185830	293959	69.71%	7.945%
24	12.204	3459	3472	3479	rBV6	2608	4513	1.07%	0.122%
25	12.297	3492	3501	3513	rBV2	14909	23299	5.53%	0.630%
26	12.625	3596	3603	3613	rVB7	3968	5508	1.31%	0.149%




Sum of corrected areas: 3700044

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030526.D
Acq On : 12 Apr 2023 18:36
Operator : SY/MD
Sample : 02275-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

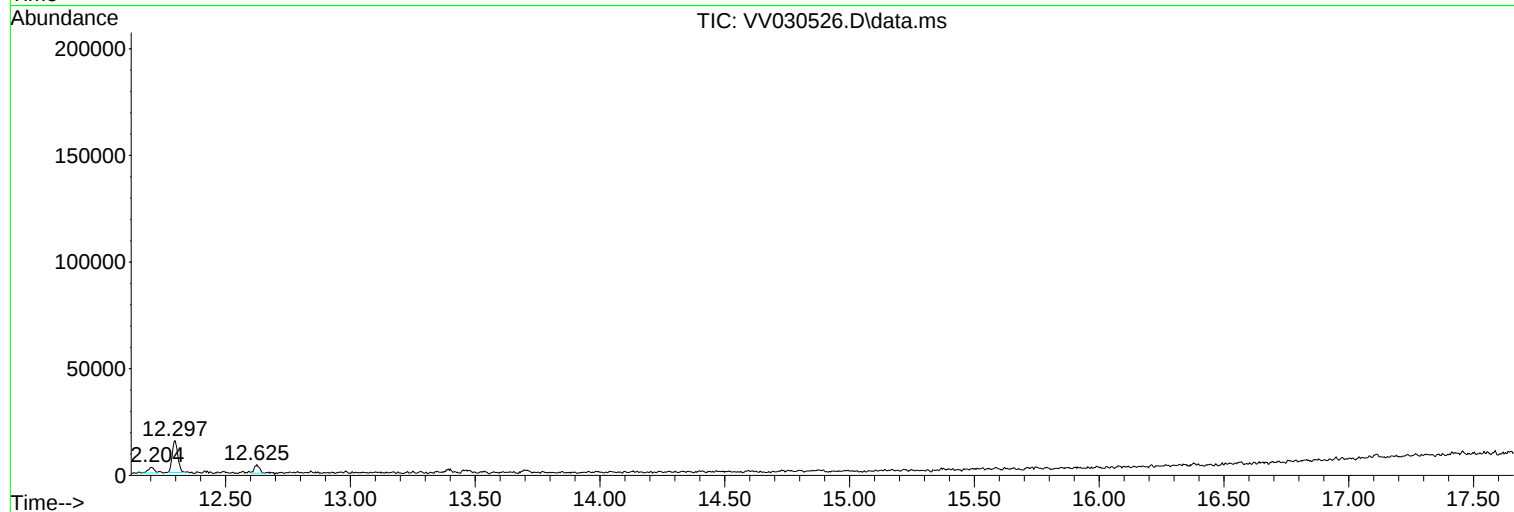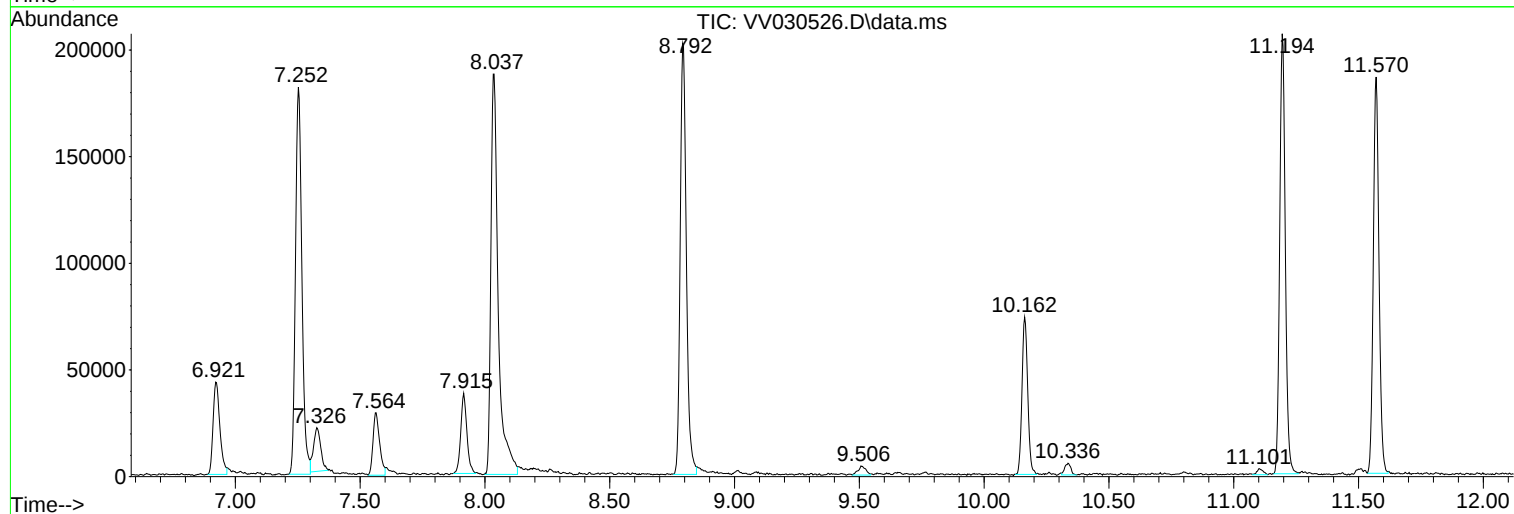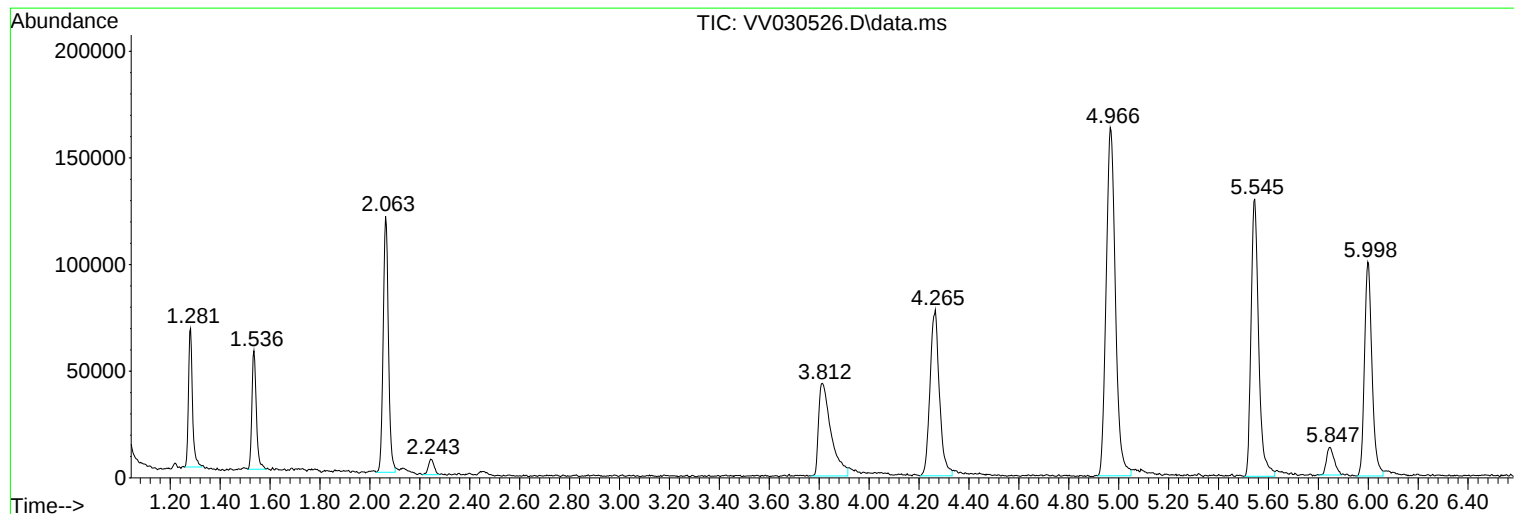

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030526.D
Acq On : 12 Apr 2023 18:36
Operator : SY/MD
Sample : 02275-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030526.D
Acq On : 12 Apr 2023 18:36
Operator : SY/MD
Sample : 02275-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------