

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
 Data File : VV030528.D
 Acq On : 12 Apr 2023 19:25
 Operator : SY/MD
 Sample : 02275-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rBV	68894	75660	18.54%	2.207%
2	1.536	147	154	168	rVB	56442	67093	16.44%	1.957%
3	2.063	308	318	333	rBV	125236	182111	44.62%	5.313%
4	3.825	855	866	902	rBV	34478	136171	33.36%	3.973%
5	4.262	984	1002	1025	rBV2	72204	189464	46.42%	5.528%
6	4.970	1204	1222	1244	rBV3	158003	408151	100.00%	11.908%
7	5.545	1387	1401	1425	rBV	129958	276960	67.86%	8.080%
8	5.847	1485	1495	1502	rBV10	2815	5468	1.34%	0.160%
9	5.998	1528	1542	1559	rBV2	92960	195452	47.89%	5.702%
10	6.924	1818	1830	1842	rBV	41262	79919	19.58%	2.332%
11	7.252	1919	1932	1949	rBV	177649	318900	78.13%	9.304%
12	7.564	2019	2029	2044	rBV	26170	48701	11.93%	1.421%
13	7.918	2129	2139	2149	rVB6	9401	18752	4.59%	0.547%
14	8.037	2165	2176	2212	rBV	177335	368511	90.29%	10.751%
15	8.793	2401	2411	2428	rBV	197057	335921	82.30%	9.801%
16	10.162	2827	2837	2856	rVB	70754	113556	27.82%	3.313%
17	10.336	2879	2891	2900	rBV4	5901	9918	2.43%	0.289%
18	11.194	3147	3158	3173	rBV	200308	313299	76.76%	9.141%
19	11.571	3262	3275	3291	rBV	170440	278331	68.19%	8.120%
20	12.297	3494	3501	3507	rBV7	3475	5220	1.28%	0.152%




Sum of corrected areas: 3427558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030528.D
Acq On : 12 Apr 2023 19:25
Operator : SY/MD
Sample : 02275-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

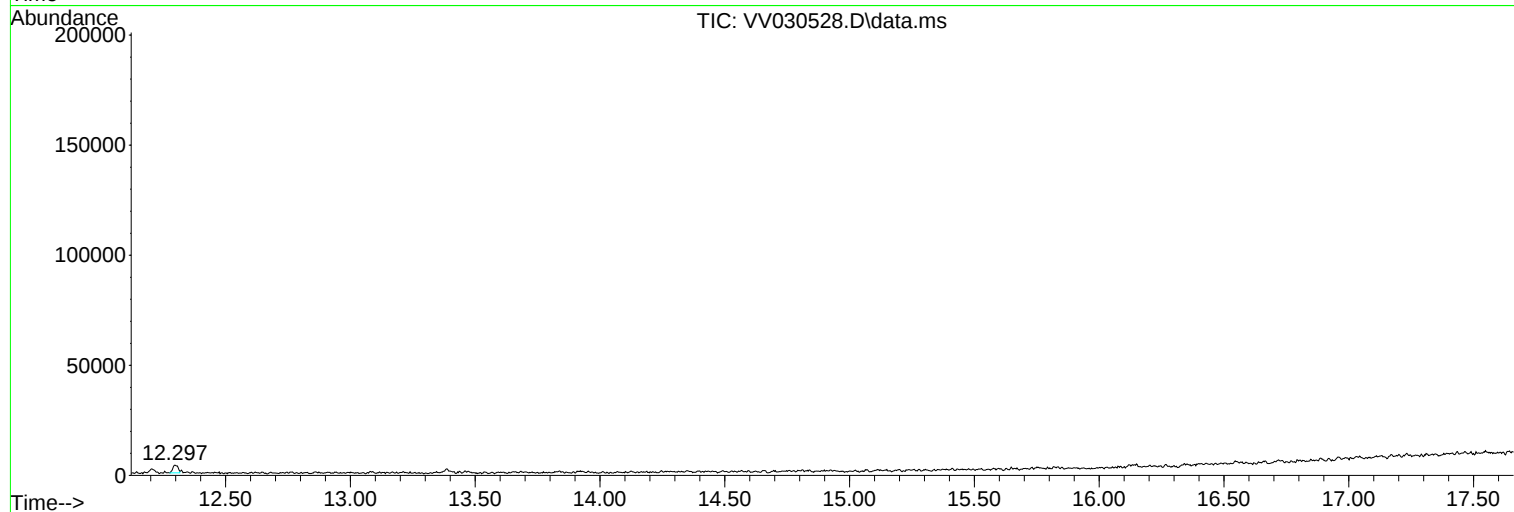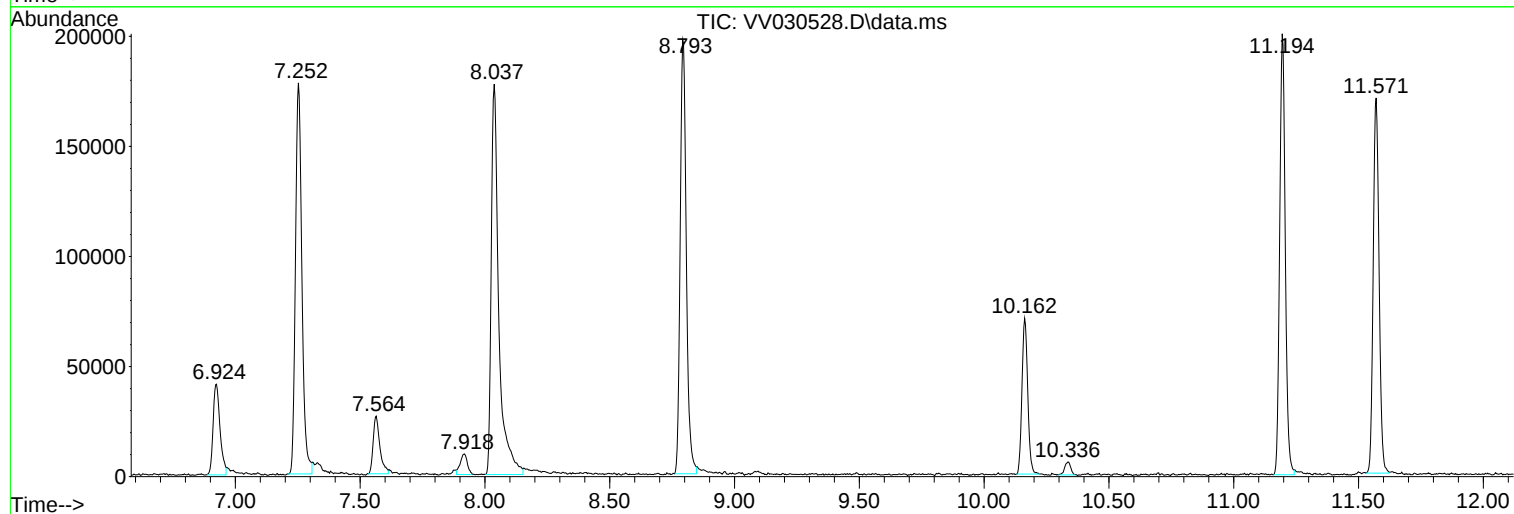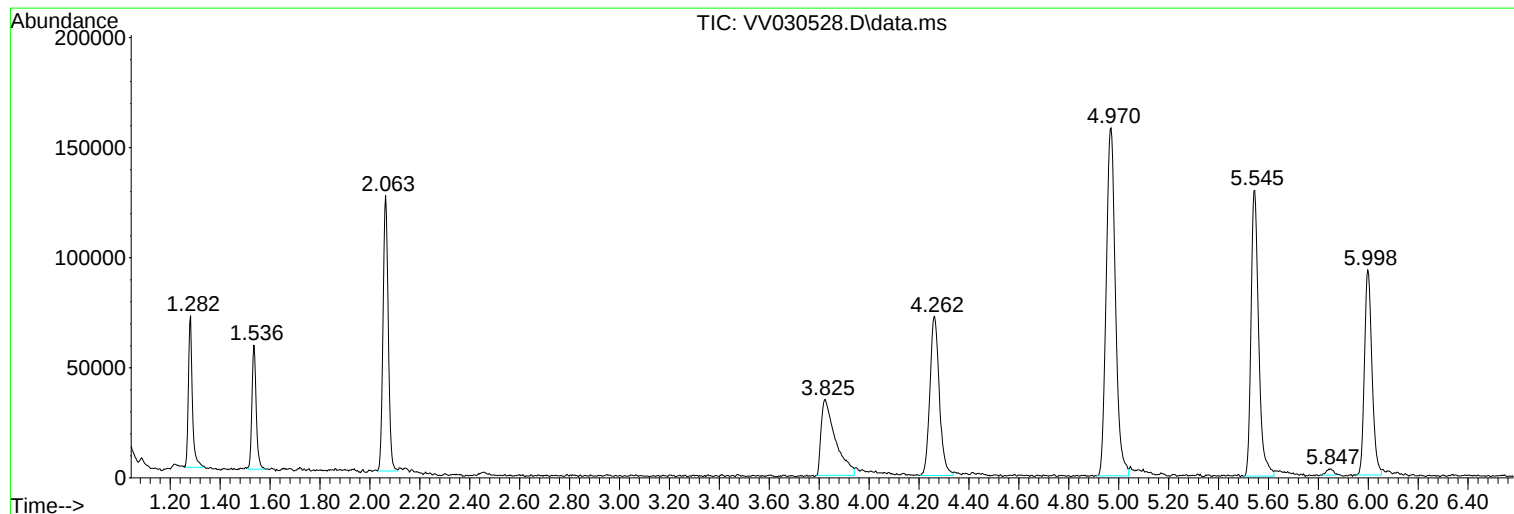

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030528.D
Acq On : 12 Apr 2023 19:25
Operator : SY/MD
Sample : 02275-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
Data File : VV030528.D
Acq On : 12 Apr 2023 19:25
Operator : SY/MD
Sample : 02275-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------