
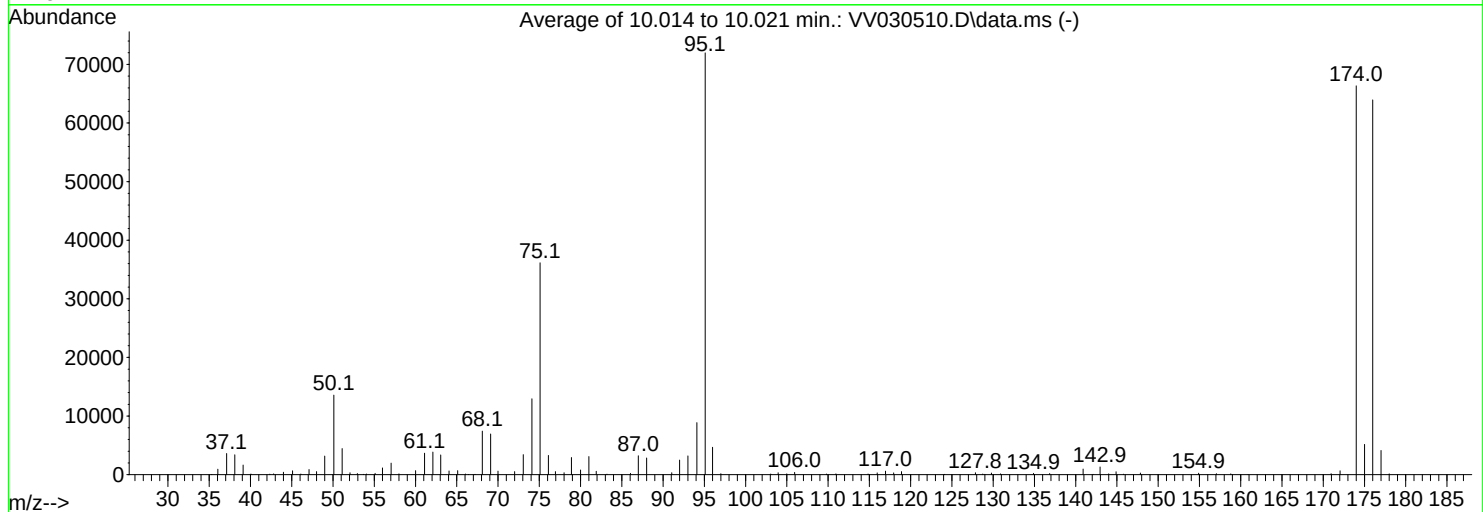


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041223\
 Data File : VV030510.D
 Acq On : 12 Apr 2023 08:56
 Operator : SY/MD
 Sample : BFB247
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB247

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Apr 14 05:16:37 2023

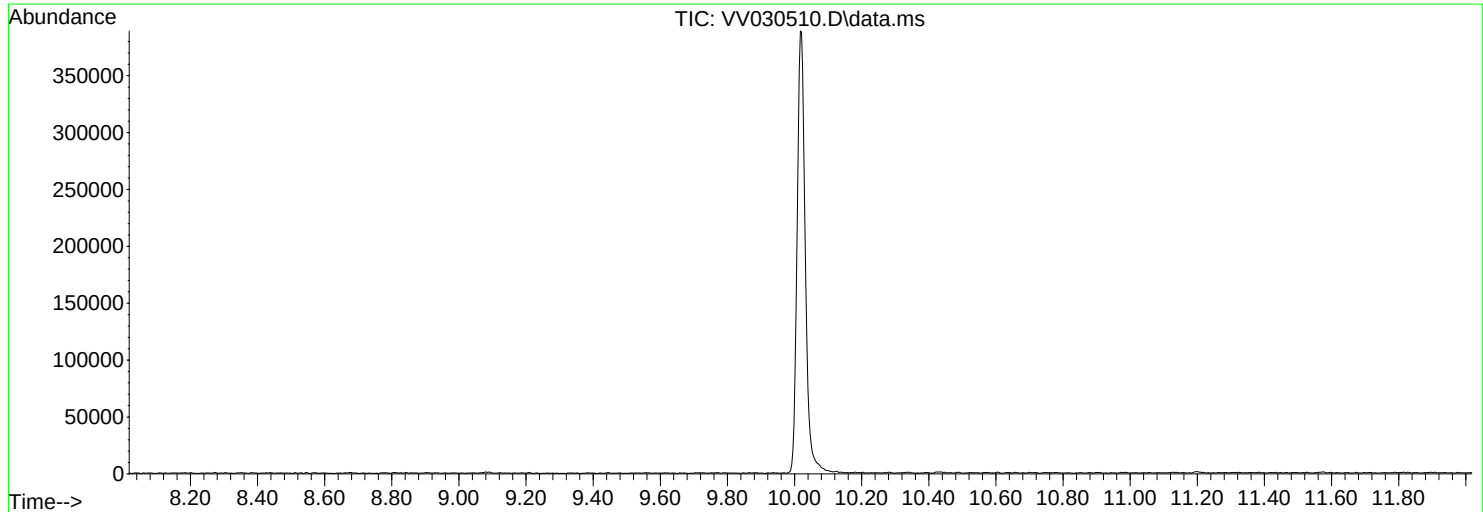

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	13563	PASS
75	95	30	80	50.2	36144	PASS
95	95	100	100	100.0	71976	PASS
96	95	5	9	6.5	4667	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.2	66347	PASS
175	174	5	9	7.8	5172	PASS
176	174	95	105	96.4	63941	PASS
177	176	5	10	6.4	4123	PASS

m/z	Abundance
35.70	136.0
40.20	140.0
44.00	245.0
46.40	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
36.10	856.0
37.10	3525.0
38.10	3239.0
39.10	1464.0
40.00	255.0
42.80	141.0
44.00	675.0
45.10	577.0
46.40	136.0
47.10	887.0
48.00	512.0
49.00	2854.0
50.10	12691.0
51.10	4190.0
52.00	313.0
52.90	158.0
53.70	142.0
54.10	134.0
55.10	230.0
56.00	1171.0
57.00	1986.0
58.00	179.0
60.00	651.0
61.10	3454.0
62.10	3606.0
63.00	3145.0
64.00	576.0
65.10	617.0
66.00	104.0
67.20	199.0
68.10	7055.0
69.10	6796.0
70.00	602.0
72.00	475.0
73.00	3324.0
74.10	12572.0
75.10	34024.0
76.10	3123.0
76.90	419.0
78.00	221.0
78.90	2835.0
80.00	777.0
81.00	2856.0
81.90	491.0
86.10	215.0
87.00	2960.0
88.00	2608.0
91.00	296.0
92.00	2326.0
93.00	3009.0
94.10	8287.0
95.10	68584.0
96.00	4514.0
97.00	152.0
103.10	100.0
103.90	319.0
105.00	148.0
106.00	362.0
109.80	112.0
110.90	122.0
114.90	106.0
116.00	288.0
117.00	530.0
118.00	261.0
118.90	482.0
124.10	103.0
127.80	312.0
128.70	179.0
129.80	271.0
130.90	124.0
134.90	178.0
136.80	225.0
140.90	896.0
142.10	154.0
142.90	1244.0
144.00	132.0
144.90	453.0
145.80	124.0
147.80	274.0
154.90	210.0
157.00	115.0
158.80	155.0
170.90	170.0
172.10	553.0
174.00	61504.0
175.00	5056.0
176.00	59168.0
177.00	3913.0
178.00	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
36.00	967.0
37.10	3662.0
38.10	3509.0
39.10	1737.0
40.00	243.0
42.40	123.0
42.80	125.0
44.00	691.0
45.10	665.0
46.10	139.0
47.10	913.0
48.00	534.0
49.00	3240.0
50.10	14009.0
51.10	4621.0
52.00	328.0
52.90	186.0
54.10	120.0
55.10	219.0
56.00	1194.0
57.10	1986.0
58.00	146.0
60.00	692.0
61.10	3771.0
62.10	3950.0
63.10	3428.0
64.00	647.0
65.10	702.0
66.00	127.0
68.10	7692.0
69.10	7190.0
70.00	623.0
72.00	556.0
73.00	3517.0
74.10	13321.0
75.10	37288.0
76.10	3319.0
77.00	532.0
78.00	325.0
78.90	3006.0
80.00	831.0
81.00	3161.0
81.90	592.0
83.20	107.0
86.10	233.0
87.00	3341.0
88.00	2919.0
91.00	331.0
92.00	2599.0
93.00	3290.0
94.10	9099.0
95.10	74112.0
96.00	4809.0
97.00	164.0
103.00	114.0
104.00	332.0
105.00	136.0
106.00	397.0
109.80	108.0
110.90	133.0
114.90	104.0
115.90	320.0
117.00	623.0
118.00	313.0
118.90	548.0
124.10	103.0
127.90	350.0
128.80	156.0
129.80	280.0
130.90	133.0
134.90	231.0
136.80	189.0
140.90	976.0
143.00	1358.0
144.00	151.0
144.90	523.0
145.80	119.0
147.90	277.0
154.90	260.0
157.10	163.0
158.80	125.0
170.90	182.0
172.00	659.0
174.00	68464.0
175.00	5330.0
176.00	66032.0
177.00	4312.0
178.00	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
35.30	103.0
36.00	936.0
37.10	3592.0
38.10	3431.0
39.10	1697.0
40.00	241.0
42.30	139.0
42.80	109.0
44.10	651.0
45.10	757.0
46.10	169.0
47.10	827.0
48.00	508.0
49.00	3398.0
50.10	13989.0
51.10	4547.0
52.10	308.0
53.00	203.0
54.00	110.0
55.10	226.0
56.00	1098.0
57.10	1932.0
58.00	111.0
60.00	689.0
61.10	3797.0
62.10	4002.0
63.10	3478.0
64.10	644.0
65.10	755.0
66.10	119.0
66.40	115.0
68.10	7569.0
69.10	6801.0
70.00	611.0
72.00	535.0
73.10	3416.0
74.10	12948.0
75.10	37120.0
76.10	3379.0
77.00	624.0
78.00	406.0
78.90	2921.0
80.00	795.0
81.00	3221.0
81.90	677.0
83.20	110.0
86.00	225.0
87.00	3401.0
88.00	2979.0
91.10	377.0
92.00	2532.0
93.00	3322.0
94.10	9243.0
95.10	73232.0
96.00	4678.0
97.00	144.0
103.00	108.0
104.00	330.0
105.00	113.0
105.90	419.0
109.80	106.0
111.00	149.0
114.80	117.0
115.90	334.0
116.90	643.0
117.90	325.0
118.90	554.0
127.90	367.0
129.00	159.0
129.80	283.0
130.90	142.0
134.90	234.0
136.90	150.0
140.90	988.0
143.00	1297.0
144.00	137.0
144.90	514.0
147.90	289.0
154.90	267.0
157.10	192.0
158.80	103.0
160.90	110.0
171.00	168.0
172.00	802.0
174.00	69072.0
175.00	5129.0
176.00	66624.0
177.00	4145.0
178.00	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247