

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035176.D
Acq On : 12 Apr 2024 16:16
Operator : SY/MD
Sample : P2056-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1




Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Manual IntegrationsAPPROVED

Quant Time: Apr 13 03:44:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

04/17/2024
Supervised By :Mahesh
Dadoda

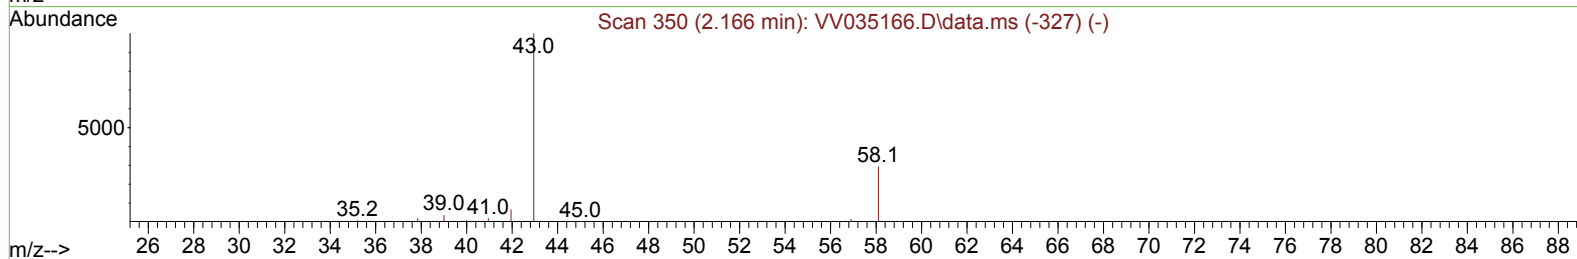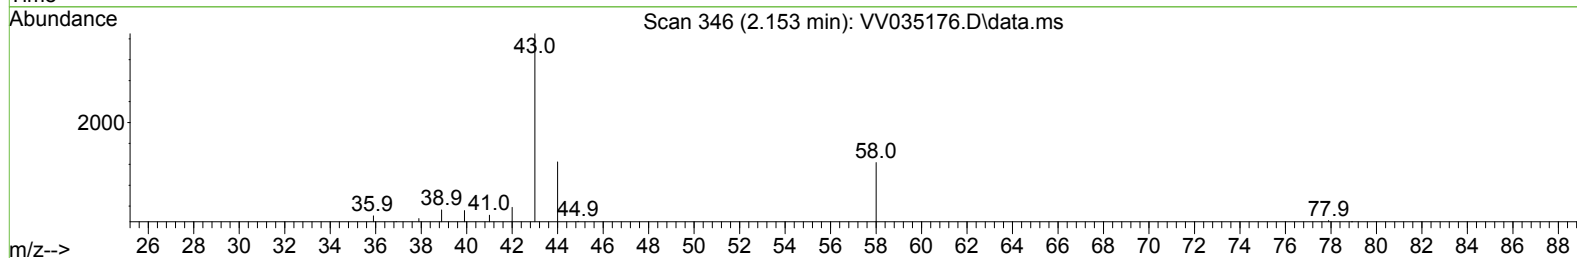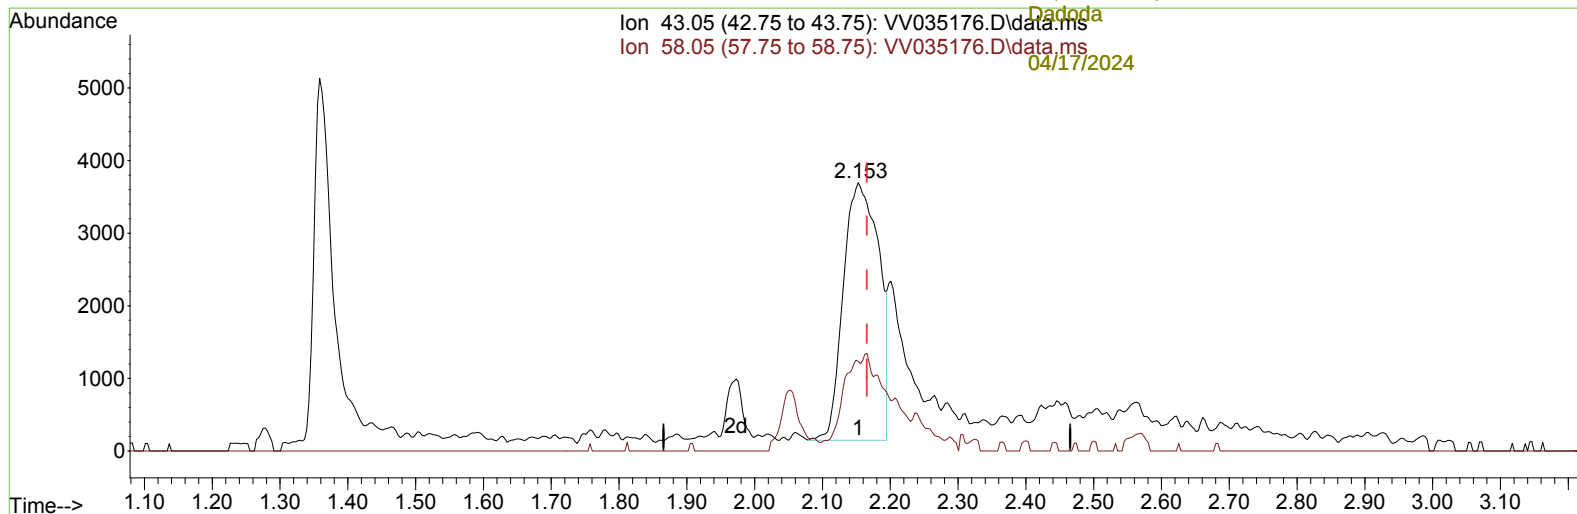

TIC: VV035176.D\data.ms

(13) Acetone (T)

2.153min (-0.013) 8.30 ug/L

response 12943

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	15.65
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035176.D
Acq On : 12 Apr 2024 16:16
Operator : SY/MD
Sample : P2056-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1




Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Manual IntegrationsAPPROVED

Quant Time: Apr 13 03:44:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

04/17/2024
Supervised By :Mahesh
Dadoda

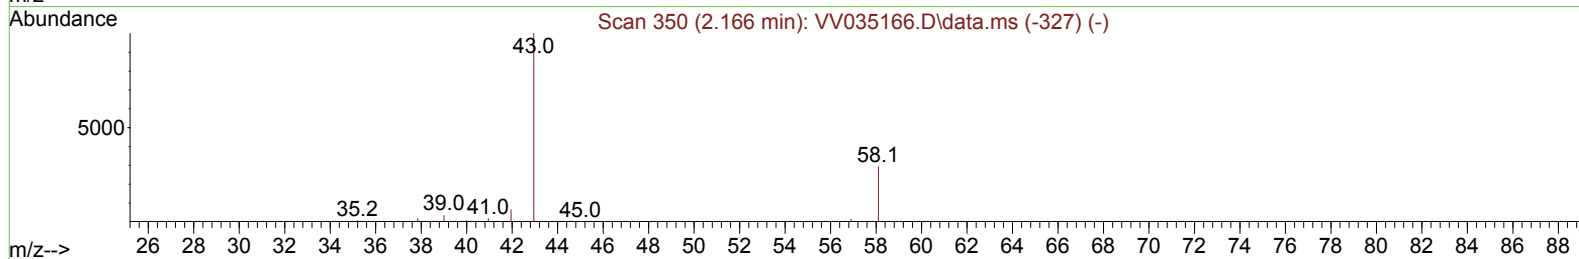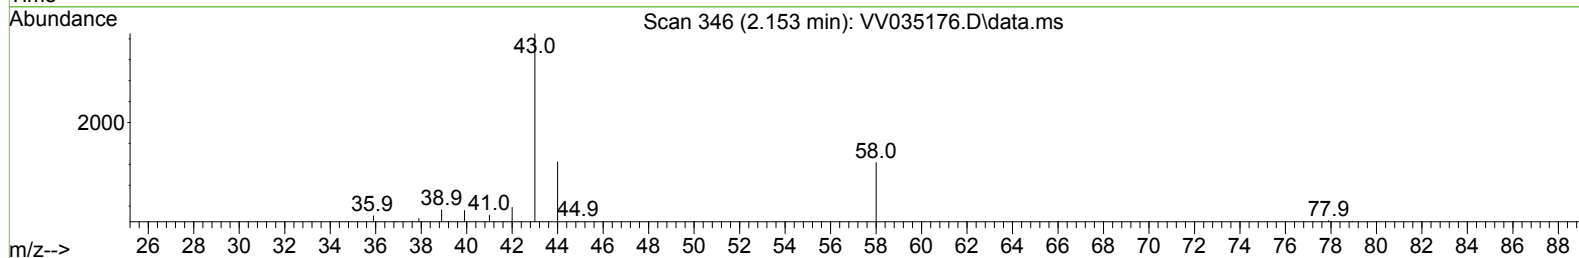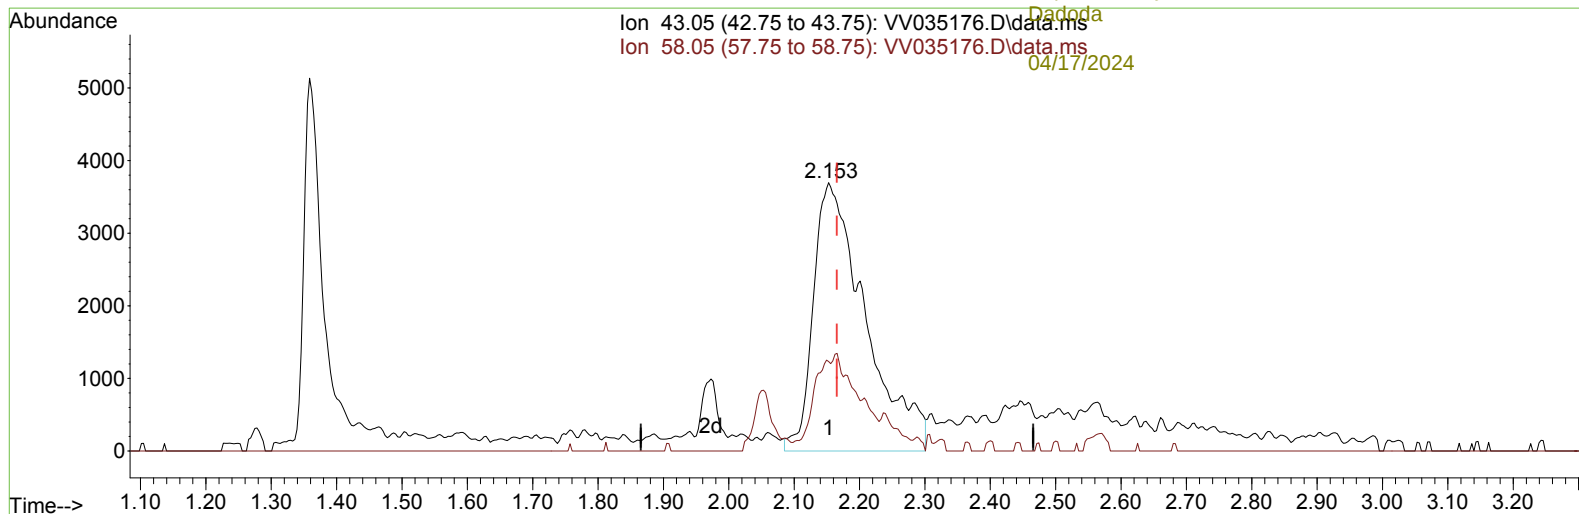

TIC: VV035176.D\data.ms

(13) Acetone (T)

2.153min (-0.013) 13.09 ug/L m

response 20421

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	9.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035176.D
 Acq On : 12 Apr 2024 16:16
 Operator : SY/MD
 Sample : P2056-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

04/17/2024
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 13 03:44:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 13 03:40:41 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		165796	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		167424	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		75130	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		44196	3.235	ug/L	0.00
Spiked Amount	5.000		Range 40 - 130	Recovery	=	64.600%	
7) Chloroethane-d5	1.532	69		47332	4.202	ug/L	0.00
Spiked Amount	5.000		Range 65 - 130	Recovery	=	84.000%	
11) 1,1-Dichloroethene-d2	2.059	65		21688	3.495	ug/L	0.00
Spiked Amount	5.000		Range 60 - 125	Recovery	=	69.800%	
20) 2-Butanone-d5	3.825	46		144193	67.446	ug/L	0.00
Spiked Amount	50.000		Range 40 - 130	Recovery	=	134.900%#	
24) Chloroform-d	4.249	84		100049	4.525	ug/L	0.00
Spiked Amount	5.000		Range 70 - 125	Recovery	=	90.600%	
26) 1,2-Dichloroethane-d4	4.947	65		53248	5.333	ug/L	0.00
Spiked Amount	5.000		Range 70 - 130	Recovery	=	106.600%	
32) Benzene-d6	4.960	84		190136	4.341	ug/L	0.00
Spiked Amount	5.000		Range 70 - 125	Recovery	=	86.800%	
36) 1,2-Dichloropropane-d6	5.989	67		65217	5.074	ug/L	0.00
Spiked Amount	5.000		Range 60 - 140	Recovery	=	101.400%	
41) Toluene-d8	7.246	98		146438	3.681	ug/L	0.00
Spiked Amount	5.000		Range 70 - 130	Recovery	=	73.600%	
43) trans-1,3-Dichloroprop...	7.564	79		17183	3.763	ug/L	0.00
Spiked Amount	5.000		Range 55 - 130	Recovery	=	75.200%	
46) 2-Hexanone-d5	8.030	63		91115	58.139	ug/L	0.00
Spiked Amount	50.000		Range 45 - 130	Recovery	=	116.280%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84		47206	5.263	ug/L	0.00
Spiked Amount	5.000		Range 65 - 120	Recovery	=	105.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152		55811	4.716	ug/L	0.00
Spiked Amount	5.000		Range 80 - 120	Recovery	=	94.400%	
Target Compounds							
						Qvalue	
13) Acetone	2.153	43		20421m	13.094	ug/L	
47) Tetrachloroethene	7.911	164		1630	0.162	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035176.D
Acq On : 12 Apr 2024 16:16
Operator : SY/MD
Sample : P2056-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Manual IntegrationsAPPROVED

Quant Time: Apr 13 03:44:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

04/17/2024
Supervised By :Mahesh
Dadoda

04/17/2024

