

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035173.D
 Acq On : 12 Apr 2024 15:04
 Operator : SY/MD
 Sample : P2056-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP8

Quant Time: Apr 13 03:43:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 13 03:40:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	199424	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	205625	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	88241	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	43618	2.654	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	53.000%
7) Chloroethane-d5	1.532	69	46793	3.453	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.000%
11) 1,1-Dichloroethene-d2	2.060	65	21490	2.879	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.600%#
20) 2-Butanone-d5	3.822	46	85001	33.055	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	66.100%
24) Chloroform-d	4.249	84	100163	3.766	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.400%
26) 1,2-Dichloroethane-d4	4.944	65	50803	4.230	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.600%
32) Benzene-d6	4.960	84	186150	3.461	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.200%#
36) 1,2-Dichloropropane-d6	5.989	67	63046	3.994	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.800%
41) Toluene-d8	7.246	98	145096	2.970	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	59.400%#
43) trans-1,3-Dichloroprop...	7.561	79	15936	2.842	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	56.800%
46) 2-Hexanone-d5	8.027	63	89600	46.551	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.100%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	47753	4.335	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	57161	4.113	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	82.200%
Target Compounds						Qvalue
47) Tetrachloroethene	7.902	164	198716	16.125	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035173.D
Acq On : 12 Apr 2024 15:04
Operator : SY/MD
Sample : P2056-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP8


Quant Time: Apr 13 03:43:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

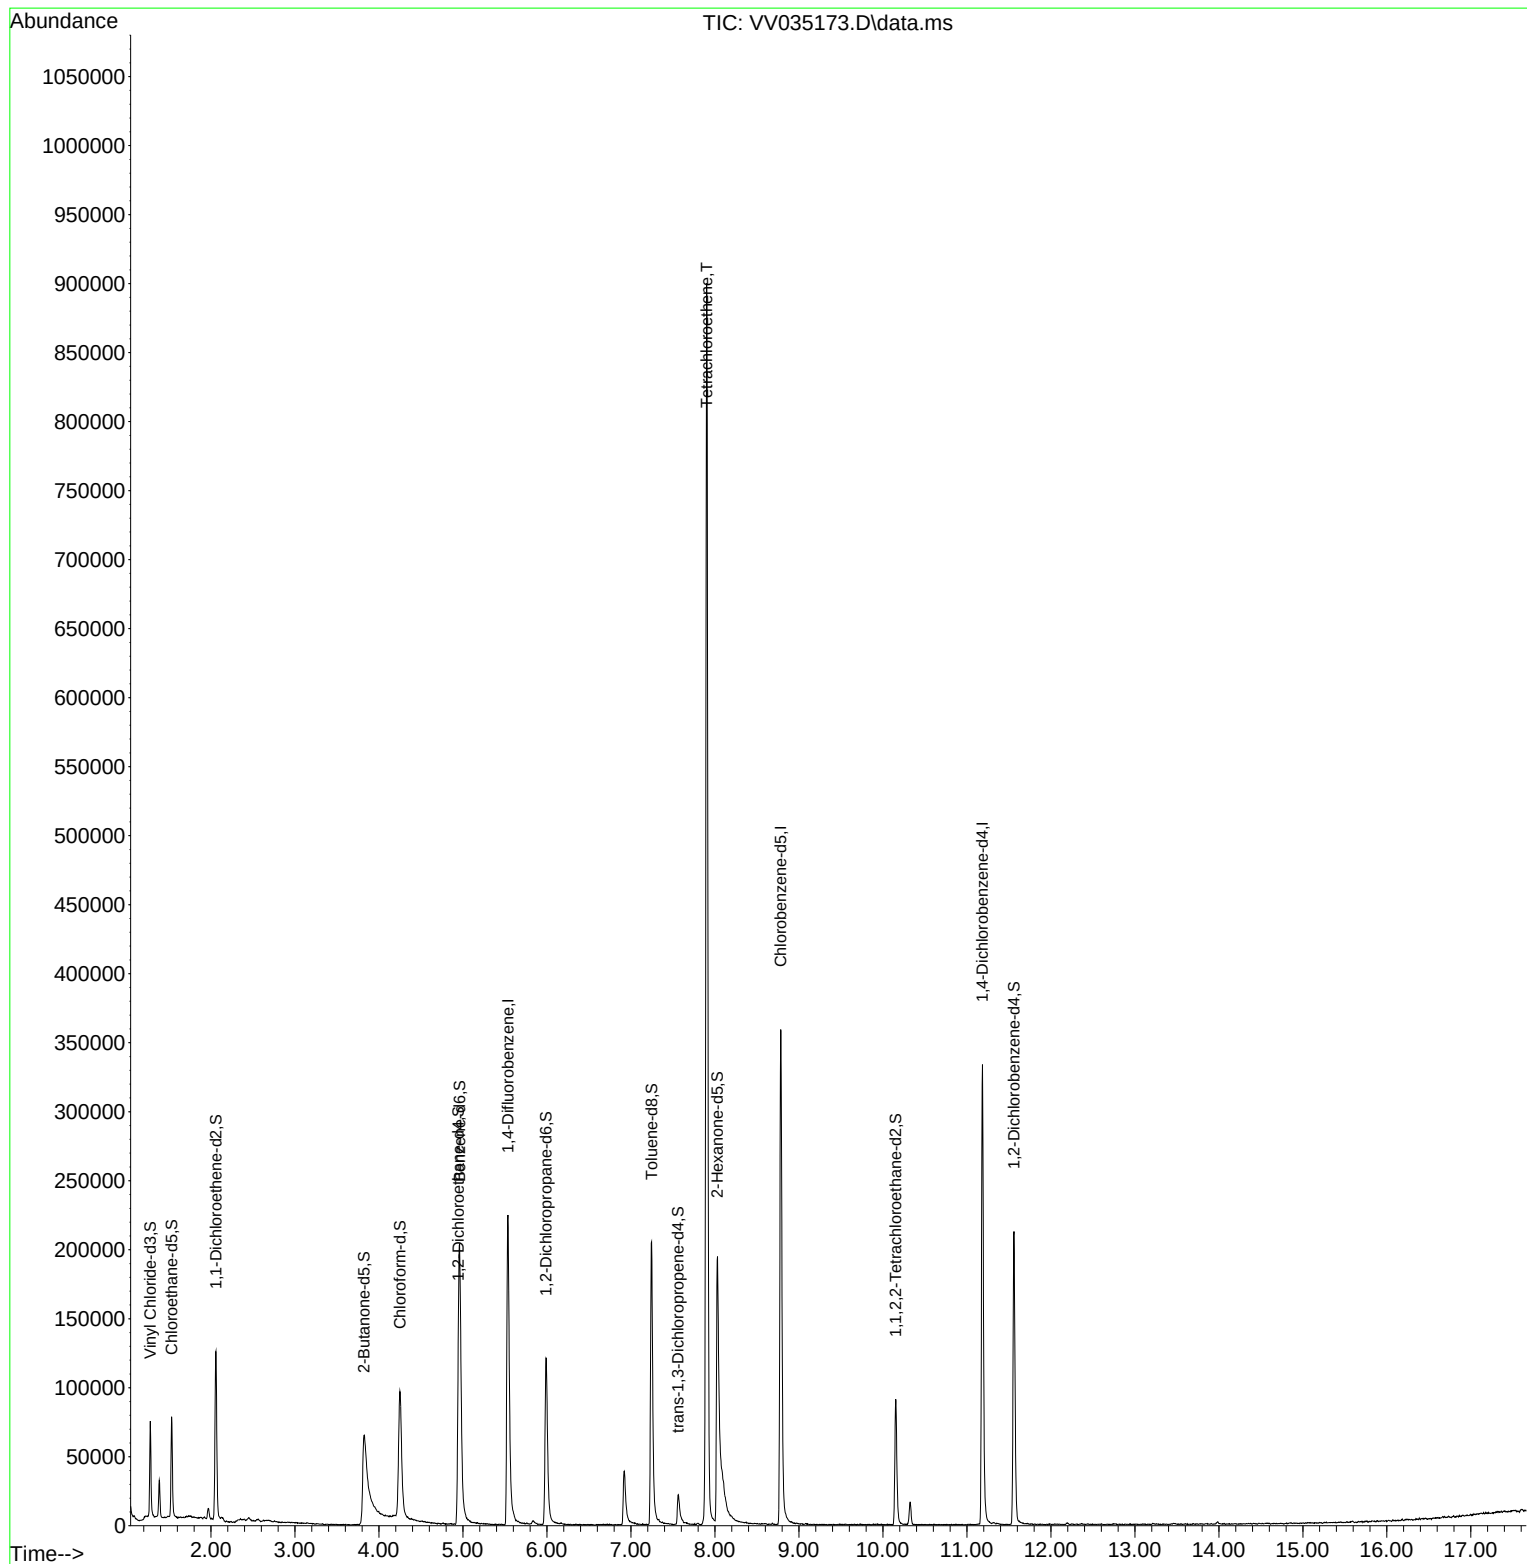

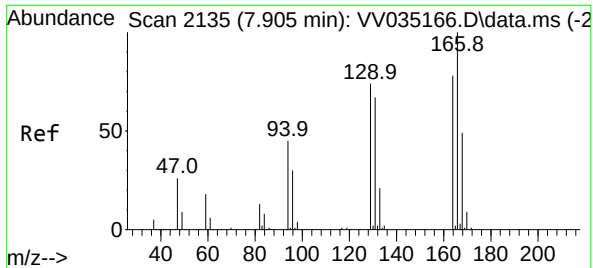

#47
 Tetrachloroethene
 Concen: 16.125 ug/L
 RT: 7.902 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: VV035173.D
 Acq: 12 Apr 2024 15:04

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP8

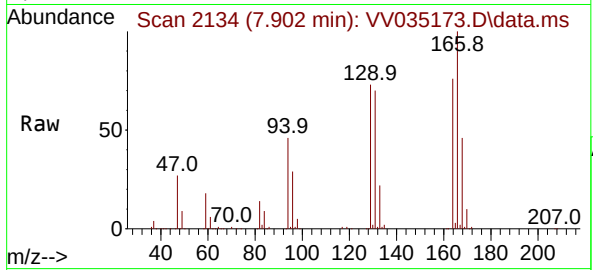

Tgt Ion:	164	Resp:	198716
Ion	Ratio	Lower	Upper
164	100		
129	95.7	66.0	122.6
131	91.7	63.0	117.0
166	130.8	91.9	170.7

