

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035179.D
 Acq On : 12 Apr 2024 17:28
 Operator : SY/MD
 Sample : P2057-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBMO

Quant Time: Apr 13 03:45:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 13 03:40:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	162634	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	169378	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	73382	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	48722	3.635	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.800%
7) Chloroethane-d5	1.532	69	51411	4.652	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	2.056	65	24147	3.967	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.400%
20) 2-Butanone-d5	3.828	46	154579	73.710	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	147.420%#
24) Chloroform-d	4.249	84	114206	5.266	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.400%
26) 1,2-Dichloroethane-d4	4.947	65	59847	6.111	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.200%
32) Benzene-d6	4.960	84	212998	4.807	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
36) 1,2-Dichloropropane-d6	5.989	67	73867	5.680	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.600%
41) Toluene-d8	7.246	98	165070	4.101	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.000%
43) trans-1,3-Dichloroprop...	7.561	79	17959	3.888	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.800%
46) 2-Hexanone-d5	8.030	63	108566	68.475	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	136.960%#
56) 1,1,2,2-Tetrachloroeth...	10.152	84	55683	6.137	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	122.800%#
66) 1,2-Dichlorobenzene-d4	11.561	152	64592	5.588	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.800%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.911	164	2190	0.216	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035179.D
Acq On : 12 Apr 2024 17:28
Operator : SY/MD
Sample : P2057-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBM0


Quant Time: Apr 13 03:45:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

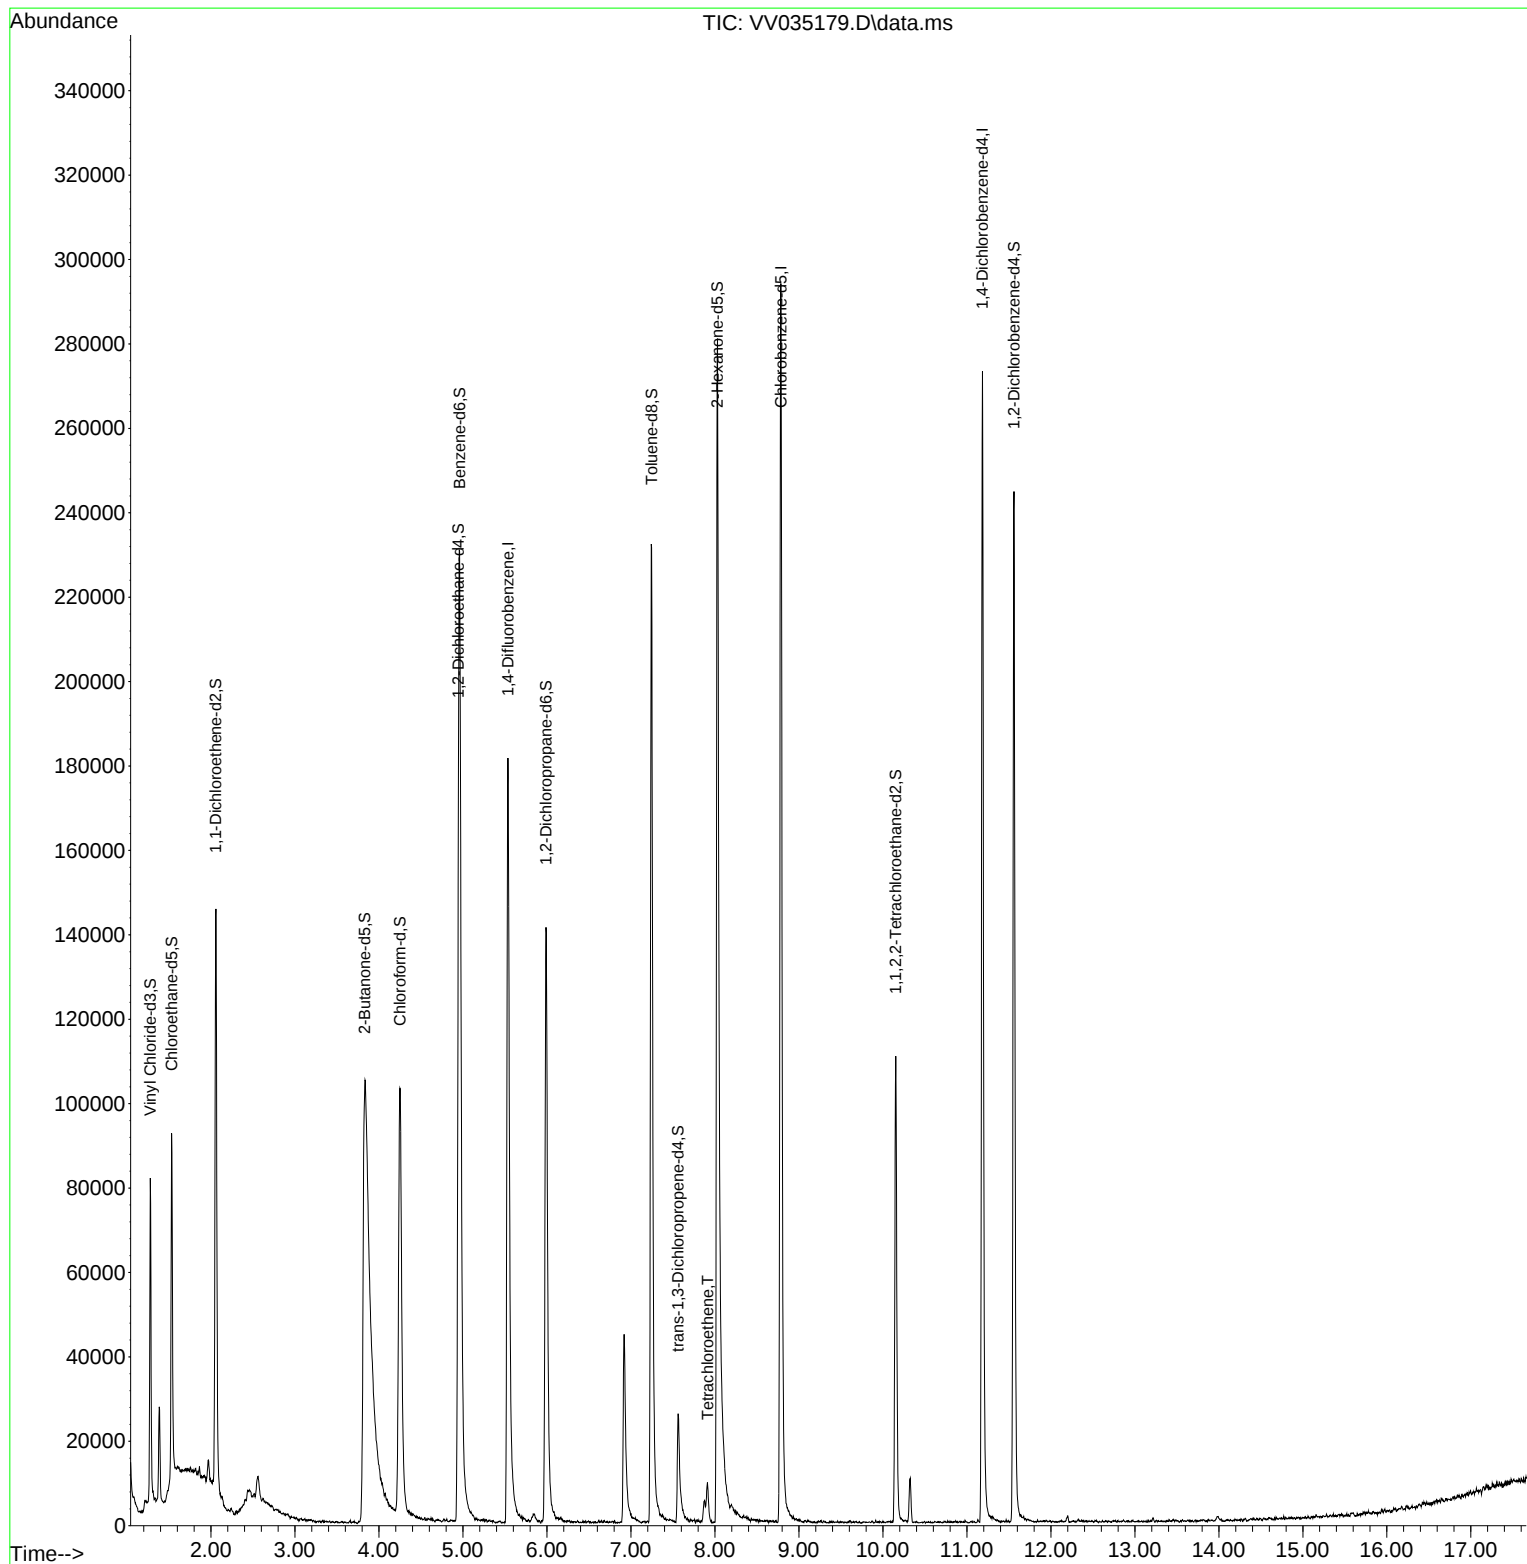

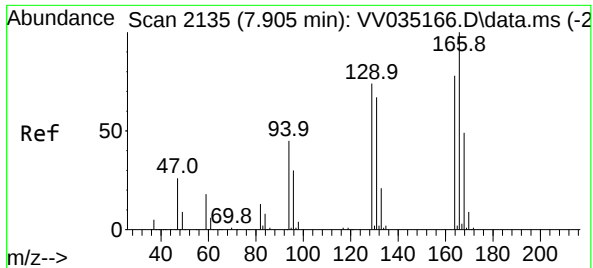

#47
 Tetrachloroethene
 Concen: 0.216 ug/L
 RT: 7.911 min Scan# 2137
 Delta R.T. 0.006 min
 Lab File: VV035179.D
 Acq: 12 Apr 2024 17:28

Instrument :
 MSVOA_V
 ClientSampleId :
 COBM0

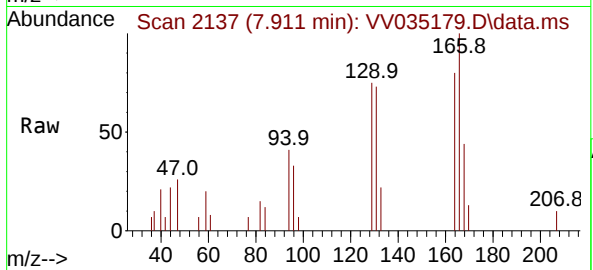

Tgt Ion:164 Resp: 2190

Ion	Ratio	Lower	Upper
164	100		
129	93.8	66.0	122.6
131	90.9	63.0	117.0
166	124.5	91.9	170.7

