

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035181.D
 Acq On : 12 Apr 2024 18:16
 Operator : SY/MD
 Sample : P2057-06DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BL7DL

Quant Time: Apr 13 03:45:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 13 03:40:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	164863	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	170031	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	73695	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	45188	3.326	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	66.600%	
7) Chloroethane-d5	1.532	69	47953	4.281	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.600%	
11) 1,1-Dichloroethene-d2	2.056	65	22992	3.726	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	74.600%	
20) 2-Butanone-d5	3.838	46	134887	63.450	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	126.900%	
24) Chloroform-d	4.246	84	109256	4.970	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.400%	
26) 1,2-Dichloroethane-d4	4.944	65	56128	5.653	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	113.000%	
32) Benzene-d6	4.960	84	201921	4.540	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.800%	
36) 1,2-Dichloropropane-d6	5.989	67	69064	5.291	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	105.800%	
41) Toluene-d8	7.243	98	153960	3.811	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.200%	
43) trans-1,3-Dichloroprop...	7.564	79	18123	3.908	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.200%	
46) 2-Hexanone-d5	8.030	63	109214	68.619	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	137.240%#	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	54416	5.974	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	119.400%	
66) 1,2-Dichlorobenzene-d4	11.561	152	58661	5.053	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.000%	
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.905	164	74357	7.297	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035181.D
Acq On : 12 Apr 2024 18:16
Operator : SY/MD
Sample : P2057-06DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BL7DL


Quant Time: Apr 13 03:45:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

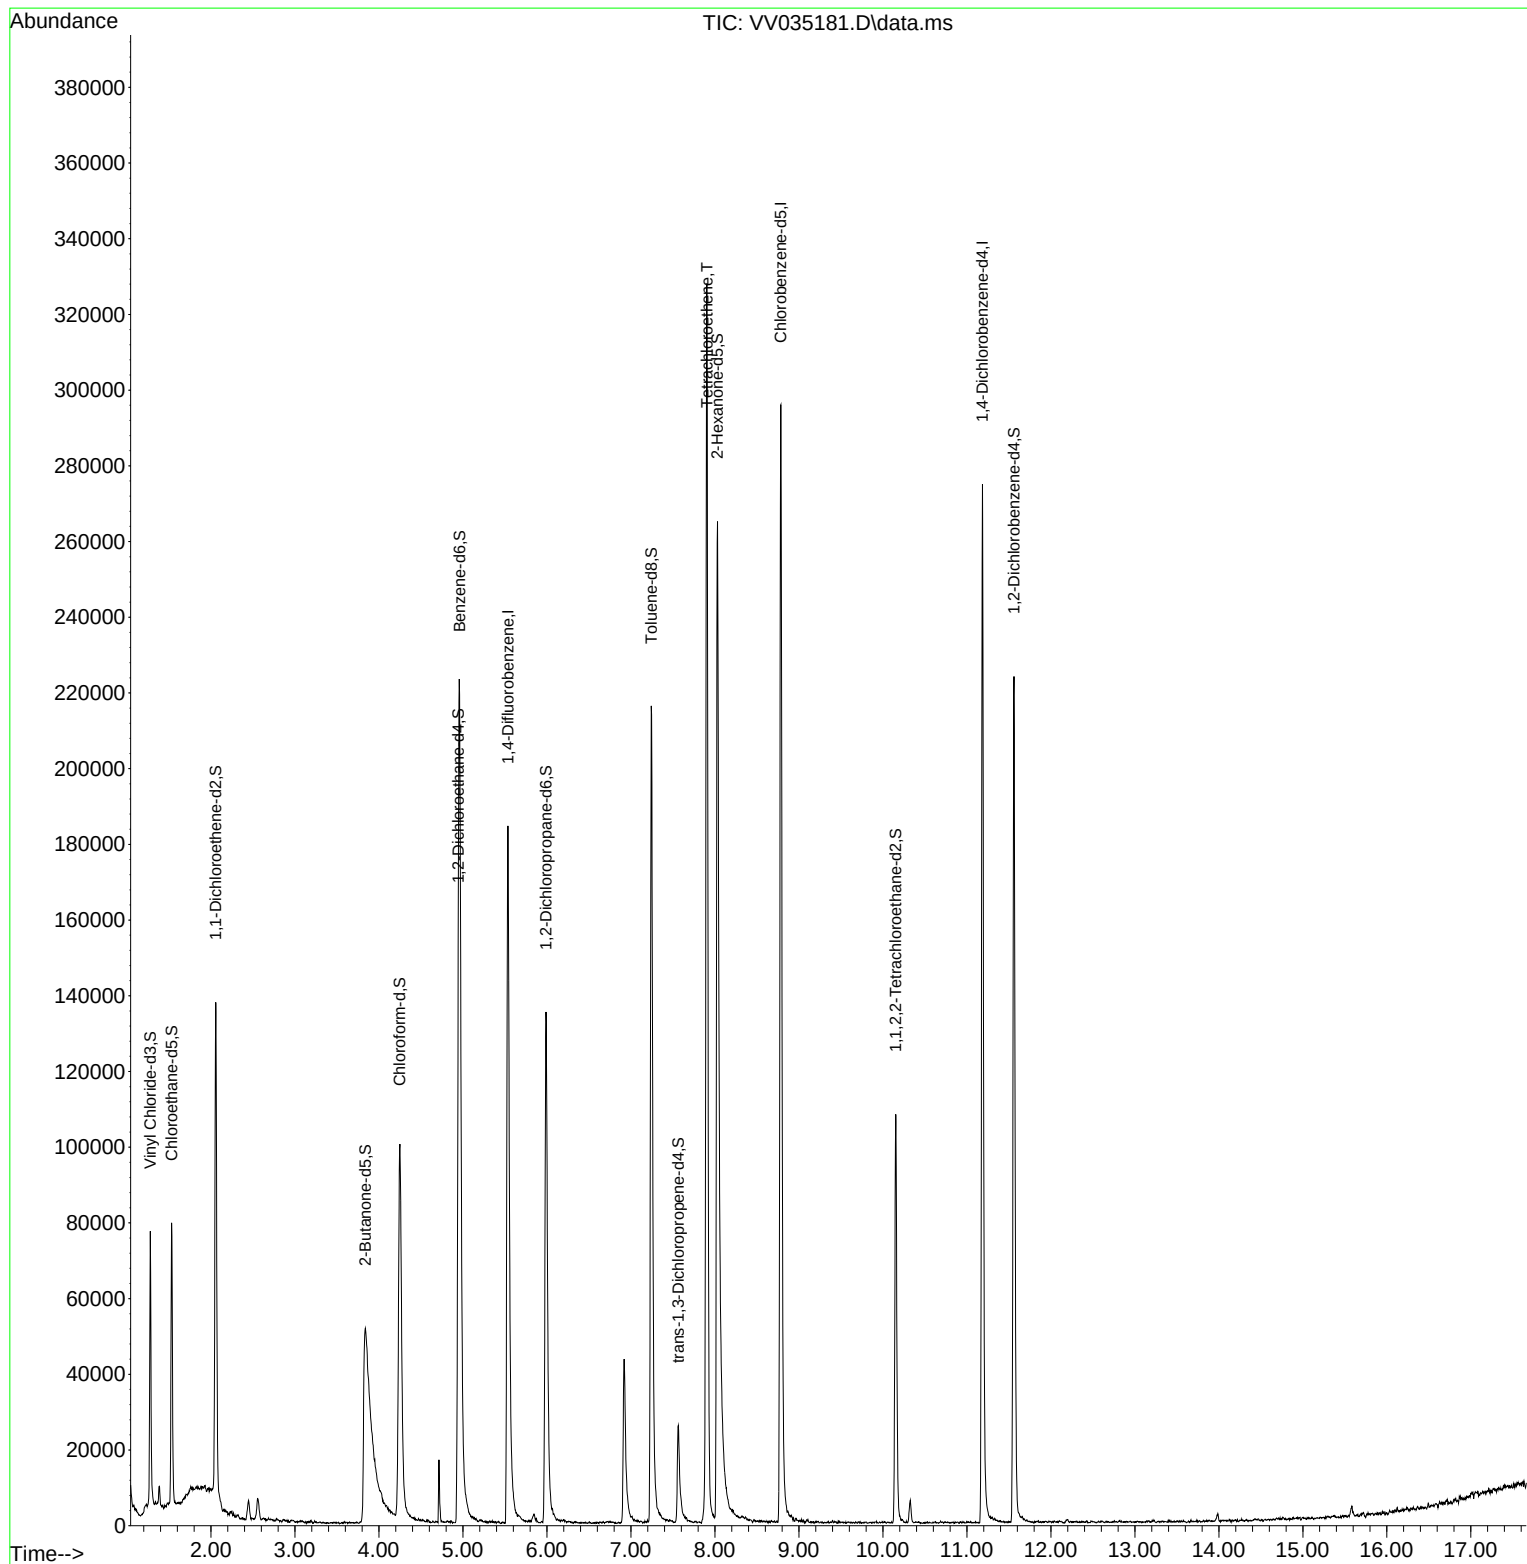

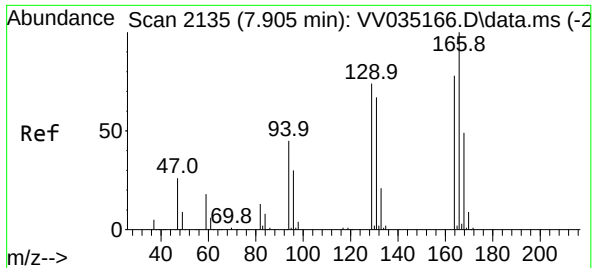

#47
 Tetrachloroethene
 Concen: 7.297 ug/L
 RT: 7.905 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VV035181.D
 Acq: 12 Apr 2024 18:16

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BL7DL

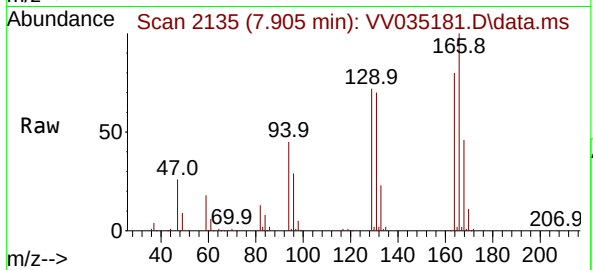

Tgt Ion:	164	Resp:	74357
Ion	Ratio	Lower	Upper
164	100		
129	90.8	66.0	122.6
131	87.7	63.0	117.0
166	125.8	91.9	170.7

