

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035185.D
 Acq On : 12 Apr 2024 19:51
 Operator : SY/MD
 Sample : P2057-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBN3

Quant Time: Apr 13 05:33:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 13 03:40:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	161890	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	168282	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.184	152	74342	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	43160	3.235	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.600%
7) Chloroethane-d5	1.532	69	47193	4.290	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.800%
11) 1,1-Dichloroethene-d2	2.059	65	21423	3.535	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.800%
20) 2-Butanone-d5	3.812	46	139500	66.825	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	133.660%#
24) Chloroform-d	4.249	84	105306	4.878	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
26) 1,2-Dichloroethane-d4	4.947	65	55441	5.687	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.800%
32) Benzene-d6	4.960	84	192212	4.366	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
36) 1,2-Dichloropropane-d6	5.989	67	66417	5.141	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.800%
41) Toluene-d8	7.246	98	151572	3.791	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.800%
43) trans-1,3-Dichloroprop...	7.564	79	16848	3.671	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.400%
46) 2-Hexanone-d5	8.027	63	99905	63.423	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	126.840%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	52832	5.861	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	117.200%
66) 1,2-Dichlorobenzene-d4	11.561	152	59030	5.041	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.240	76	5024	0.137	ug/L	95
47) Tetrachloroethene	7.908	164	24828	2.462	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035185.D
Acq On : 12 Apr 2024 19:51
Operator : SY/MD
Sample : P2057-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBN3


Quant Time: Apr 13 05:33:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

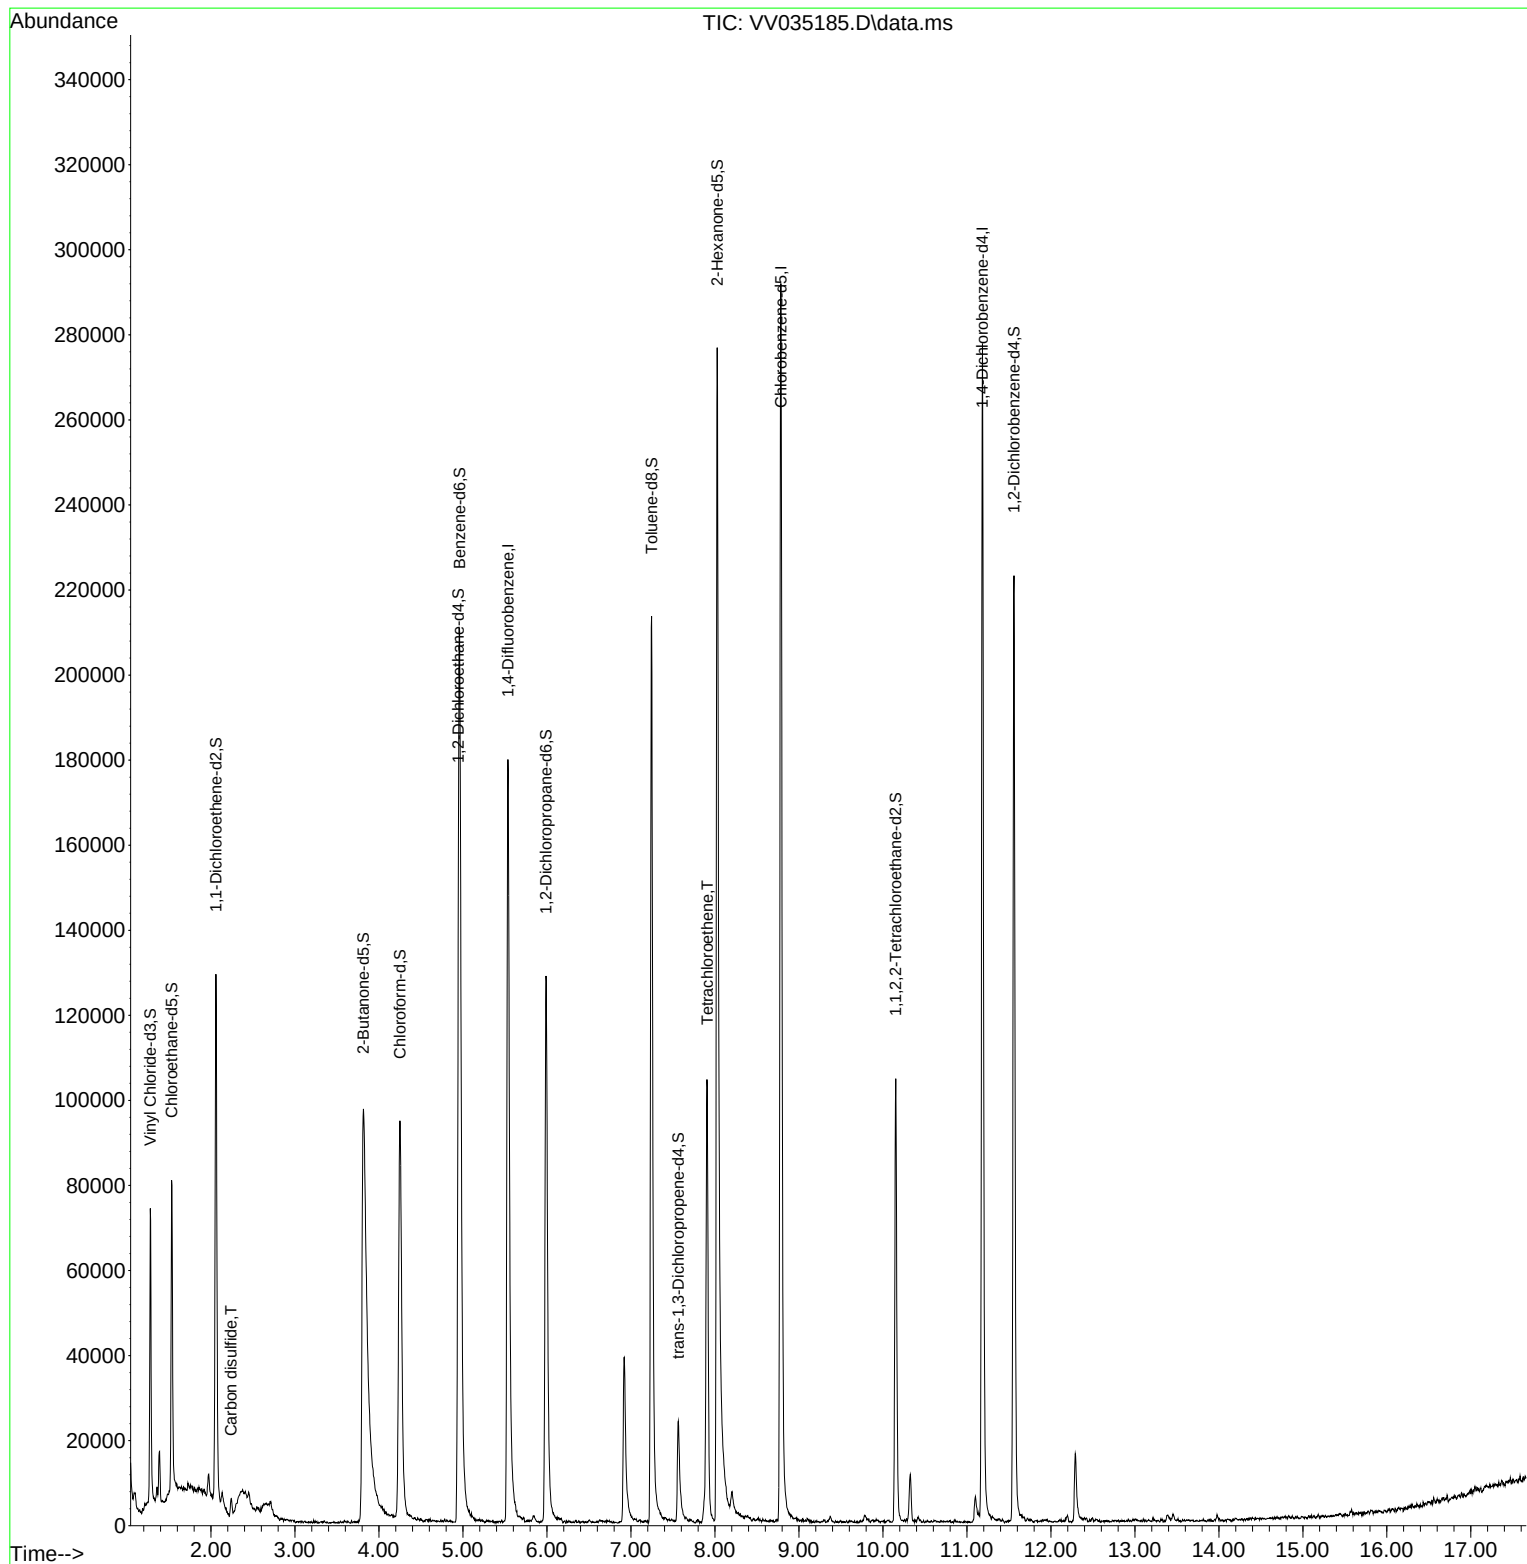



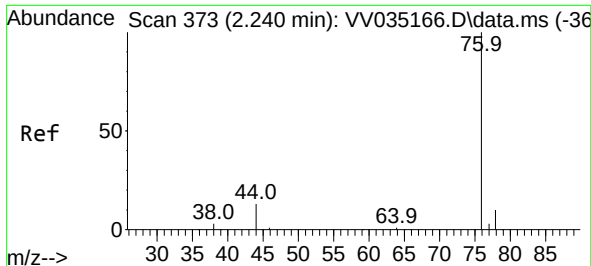


#14
Carbon disulfide
Concen: 0.137 ug/L
RT: 2.240 min Scan# 31
Delta R.T. -0.000 min
Lab File: VV035185.D
Acq: 12 Apr 2024 19:51


Instrument :
MSVOA_V
ClientSampleId :
COBN3

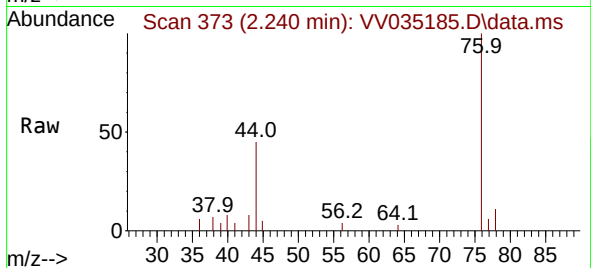

Tgt Ion: 76 Resp: 5024
Ion Ratio Lower Upper
76 100
78 11.1 7.4 11.2

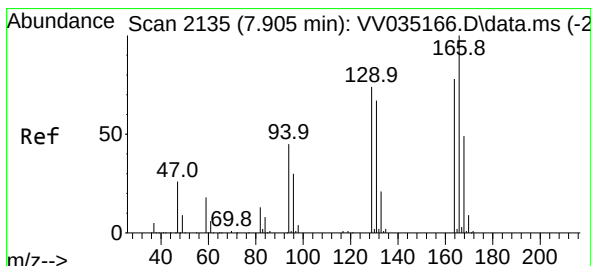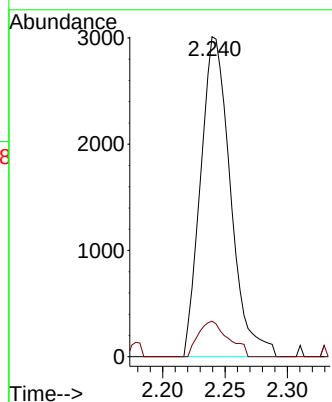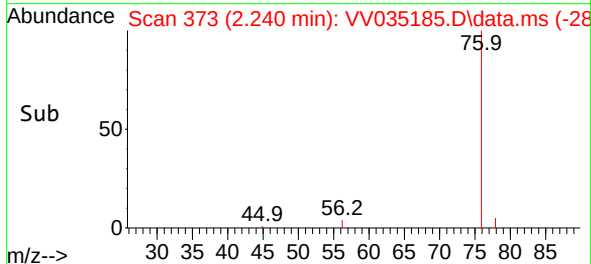

#47
Tetrachloroethene
Concen: 2.462 ug/L
RT: 7.908 min Scan# 2136
Delta R.T. 0.003 min
Lab File: VV035185.D
Acq: 12 Apr 2024 19:51

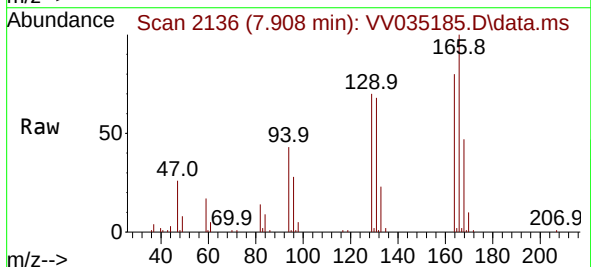

Tgt Ion: 164 Resp: 24828
Ion Ratio Lower Upper
164 100
129 87.3 66.0 122.6
131 84.9 63.0 117.0
166 125.5 91.9 170.7

