

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041224\
 Data File : VW035186.D
 Acq On : 12 Apr 2024 20:15
 Operator : SY/MD
 Sample : P2057-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BN4

Quant Time: Apr 13 05:33:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 13 03:40:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	164095	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	173082	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	74284	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	45024	3.329	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	66.600%	
7) Chloroethane-d5	1.532	69	47807	4.288	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.800%	
11) 1,1-Dichloroethene-d2	2.060	65	21510	3.502	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	70.000%	
20) 2-Butanone-d5	3.815	46	143449	67.794	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	135.580%#	
24) Chloroform-d	4.249	84	107598	4.917	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4	4.947	65	55182	5.584	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	111.600%	
32) Benzene-d6	4.960	84	196535	4.341	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.800%	
36) 1,2-Dichloropropane-d6	5.989	67	68366	5.145	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.800%	
41) Toluene-d8	7.246	98	151482	3.683	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	73.600%	
43) trans-1,3-Dichloroprop...	7.564	79	18421	3.902	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.000%	
46) 2-Hexanone-d5	8.027	63	103323	63.774	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	127.540%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	53902	5.814	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	116.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152	60049	5.132	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.600%	
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.905	164	6101	0.588	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035186.D
Acq On : 12 Apr 2024 20:15
Operator : SY/MD
Sample : P2057-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BN4


Quant Time: Apr 13 05:33:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

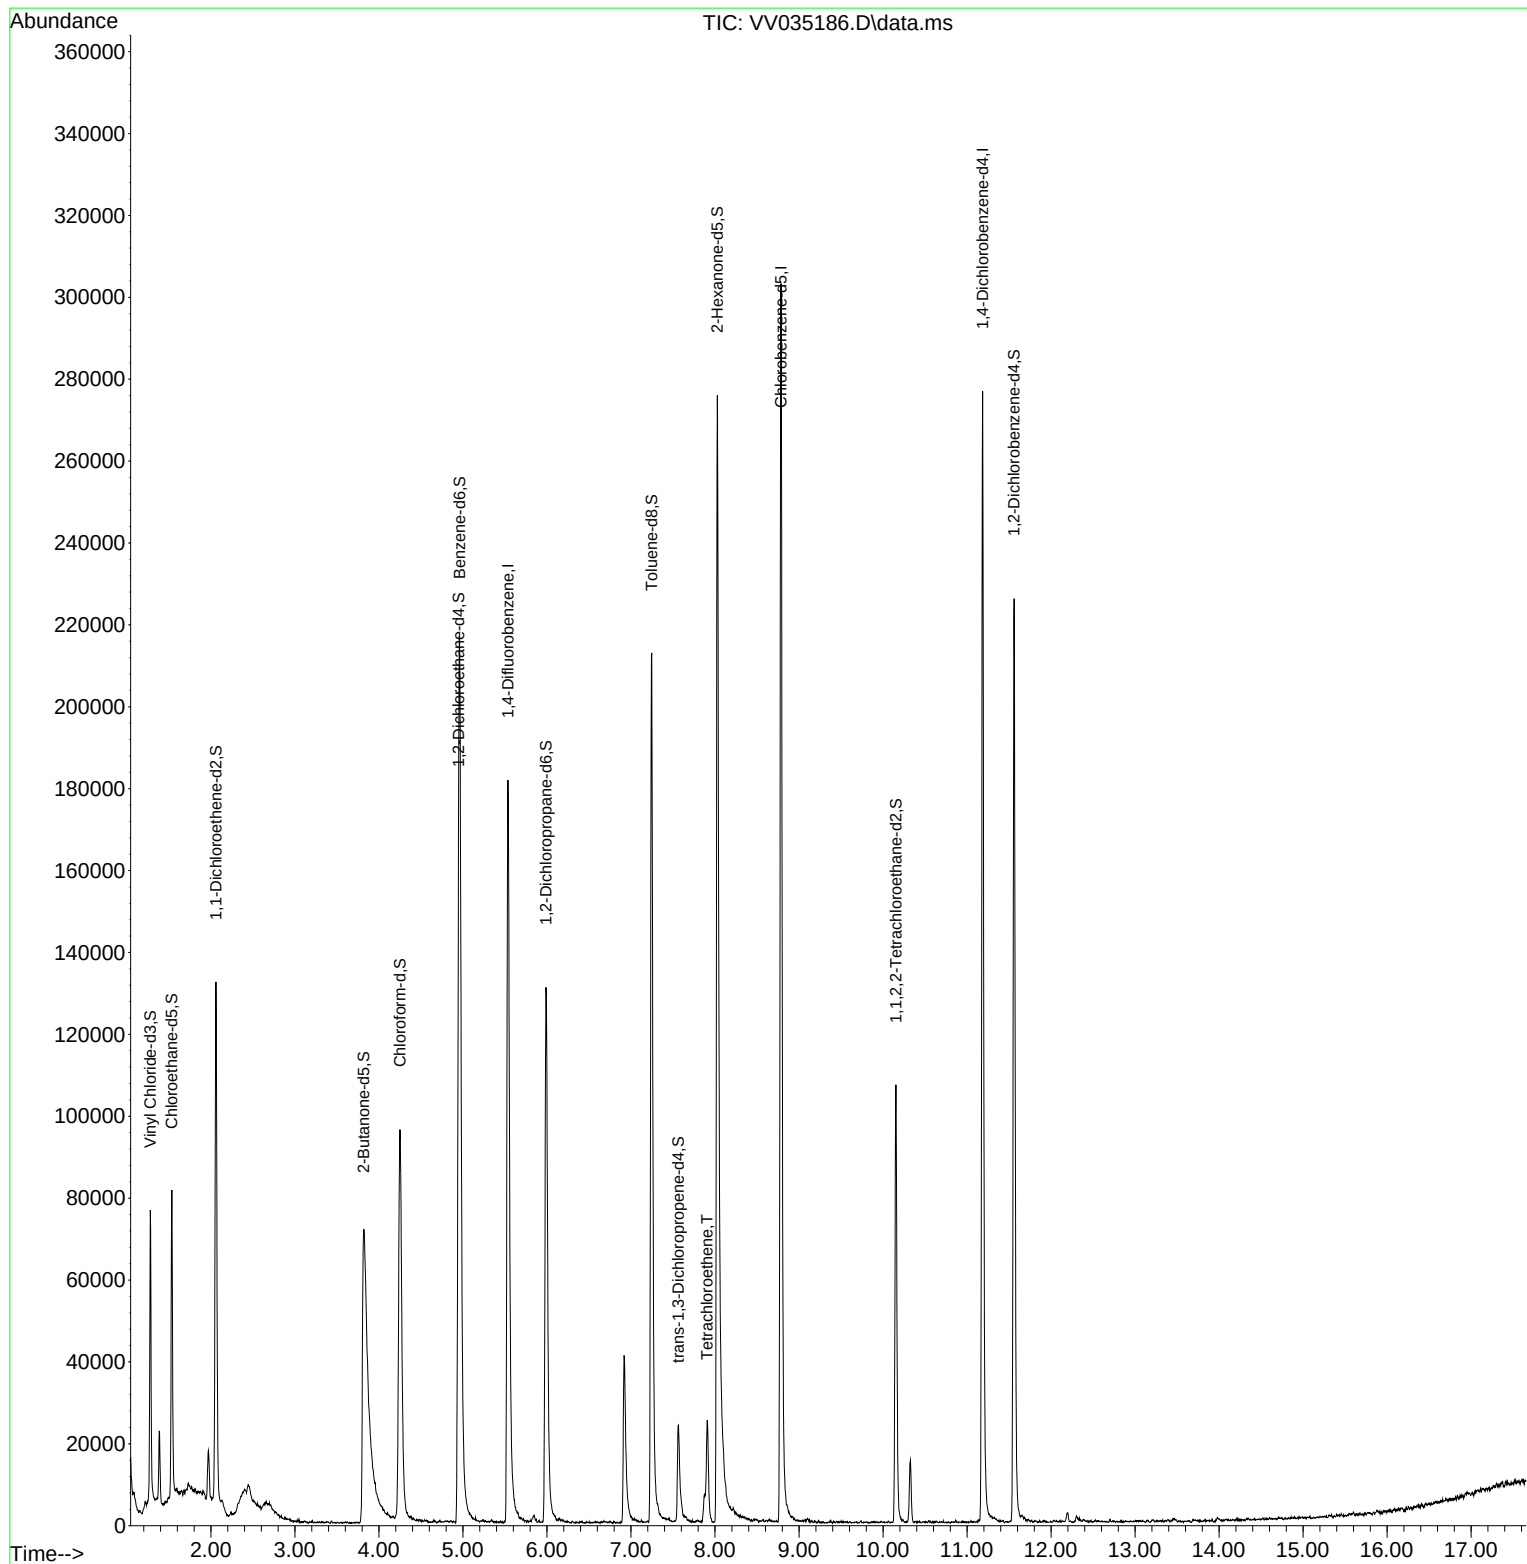

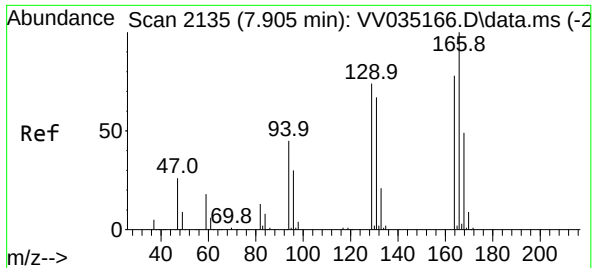

#47
 Tetrachloroethene
 Concen: 0.588 ug/L
 RT: 7.905 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VV035186.D
 Acq: 12 Apr 2024 20:15

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BN4

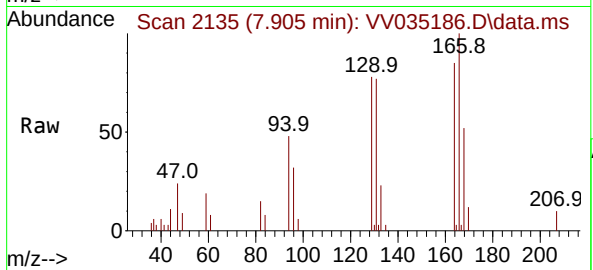

Tgt Ion:	164	Resp:	6101
Ion	Ratio	Lower	Upper
164	100		
129	89.2	66.0	122.6
131	87.6	63.0	117.0
166	113.7	91.9	170.7

