

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041224\
 Data File : VW035187.D
 Acq On : 12 Apr 2024 20:39
 Operator : SY/MD
 Sample : P2057-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP3

Quant Time: Apr 13 05:34:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 13 03:40:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	160374	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	165391	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	70941	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	43697	3.306	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.200%
7) Chloroethane-d5	1.532	69	49008	4.497	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.000%
11) 1,1-Dichloroethene-d2	2.060	65	21239	3.538	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.800%
20) 2-Butanone-d5	3.815	46	137555	66.516	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	133.040%#
24) Chloroform-d	4.249	84	107472	5.025	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	4.944	65	55965	5.795	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.800%
32) Benzene-d6	4.960	84	198853	4.596	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.000%
36) 1,2-Dichloropropane-d6	5.989	67	69234	5.452	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.000%
41) Toluene-d8	7.246	98	151319	3.850	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.000%
43) trans-1,3-Dichloroprop...	7.564	79	17216	3.817	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.400%
46) 2-Hexanone-d5	8.027	63	100898	65.173	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	130.340%#
56) 1,1,2,2-Tetrachloroeth...	10.153	84	52072	5.877	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	117.600%
66) 1,2-Dichlorobenzene-d4	11.561	152	60158	5.384	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.600%
Target Compounds						Qvalue
47) Tetrachloroethene	7.915	164	1786	0.180	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035187.D
Acq On : 12 Apr 2024 20:39
Operator : SY/MD
Sample : P2057-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP3


Quant Time: Apr 13 05:34:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 13 03:40:41 2024
Response via : Initial Calibration

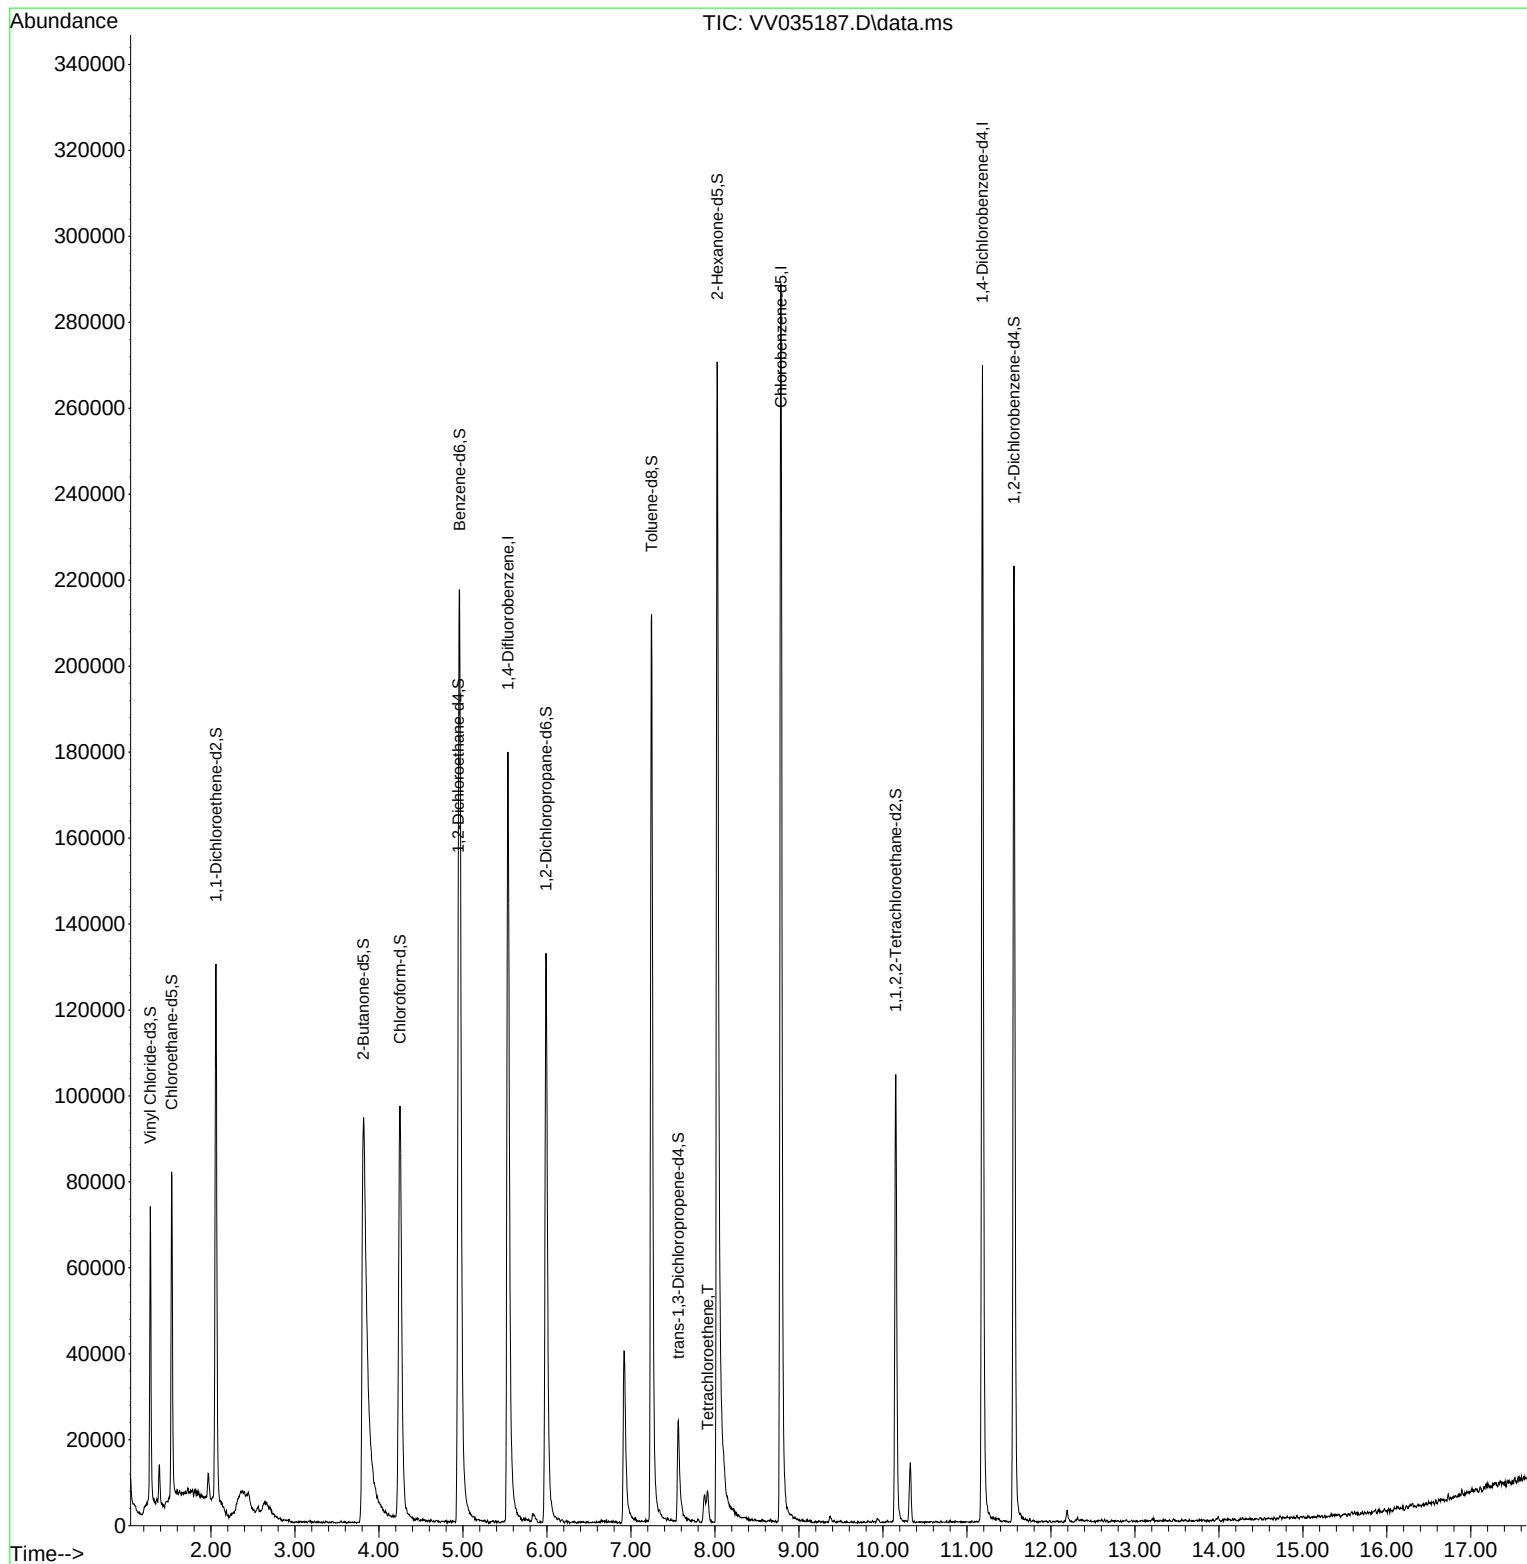

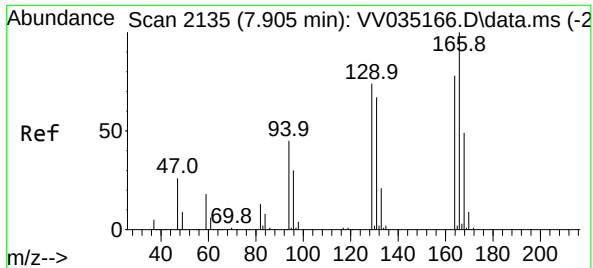

#47
 Tetrachloroethene
 Concen: 0.180 ug/L
 RT: 7.915 min Scan# 21
 Delta R.T. 0.010 min
 Lab File: VV035187.D
 Acq: 12 Apr 2024 20:39

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP3

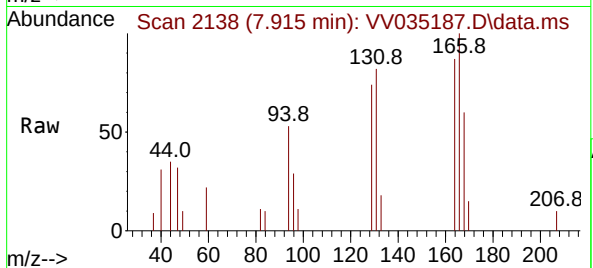

Tgt Ion:164 Resp: 1786

Ion	Ratio	Lower	Upper
164	100		
129	84.7	66.0	122.6
131	94.2	63.0	117.0
166	114.4	91.9	170.7

